

SSG6M80A Series Multi-Channel Microwave Signal Generator

Programming Guide

EN01A



SIGLENT TECHNOLOGIES CO., LTD.

Contents

1	Programming Overview	1
1.1	Build communication via VISA	1
1.1.1	Install NI-VISA	1
1.1.2	Connect the instrument to computer	5
1.2	Remote Control.....	7
1.2.1	User-defined Programming.....	7
1.2.2	Send SCPI via NI-MAX	7
1.2.3	Send SCPI over Telnet	12
1.2.4	Send SCPI over Socket	14
2	Introduction to the SCPI Language	15
2.1	Command Format	15
2.2	Symbol Instruction	15
2.3	Parameter Type.....	16
2.4	Command Abbreviation	17
3	Commands	18
3.1	IEEE 488.2 Common Commands.....	18
3.1.1	Identification Query (*IDN?)	18
3.1.2	Reset (*RST)	18
3.1.3	Clear Status (*CLS).....	18
3.1.4	Standard Event Status Enable (*ESE).....	19
3.1.5	Standard Event Status Register Query (*ESR?)	19
3.1.6	Operation Complete Query (*OPC)	19
3.1.7	Service Request Enable (*SRE)	20
3.1.8	Status Byte Query (*STB?).....	20
3.1.9	Wait-to-Continue (*WAI).....	20
3.1.10	Self Test Query (*TST?)	21
3.2	SYSTem Commands	22
3.2.1	System Configuration.....	22
3.2.2	System Reset/Preset.....	30
3.3	OUTPut Commands.....	32
3.3.1	RF Output ([:SOURce<ch>]:OUTPut)	32
3.3.2	Analog Modulation State (:OUTPut:MODulation[:STATe])	32

3.4	SOURce Commands	33
3.4.1	RF Output ([:SOURce<ch>]:OUTPut)	33
3.4.2	Software Trigger([:SOURce<ch>]:*TRG)	33
3.4.3	Frequency	33
3.4.4	Level	37
3.4.5	Sweep	45
3.4.6	Sensor	58
3.4.7	Analog Modulation	60
3.4.8	Pulse Modulation	69
3.4.9	Phase Coherence	81
3.4.10	System Preset	83
3.5	SENSe Commands	83
3.5.1	Power Sensor	83
4	Programming Examples	95
4.1	VISA Examples	95
4.1.1	VC++ Example	95
4.1.2	VB Example	102
4.1.3	MATLAB Example	107
4.1.4	LabVIEW Example	109
4.2	Socket Examples	112
4.2.1	Python Example	112

1 Programming Overview

The SSG6M80A Series Multi-Channel Signal Generator supports USB, LAN and USB-GPIB interfaces. Through these interfaces, combined with NI-VISA and corresponding programming language, users can use the command set based on SCPI (Standard Commands for Programmable Instruments) to remotely program and control the instrument, and interact with other programmable instruments that support the SCPI command set.

Through the LAN interface, VXI-11, Sockets, and Telnet protocols can be used to communicate with the instrument.

This chapter describes how to establish communication between the Multi-Channel signal generator and the computer, and how to remotely control the Multi-Channel signal generator.

1.1 Build communication via VISA

1.1.1 Install NI-VISA


Before programming, please make sure that you have properly installed the latest version of National Instruments NI-VISA Software.

NI-VISA is a communication library for communication between computers and devices. NI software has two valid VISA installation packages: full version and run-time engine version (Run-Time Engine). The runtime engine version provides NI device drivers such as USB-TMC, VXI and GPIB, etc. It is mainly used for remote control. The full version includes the runtime engine and NI MAX tools, where NI MAX is the user interface for controlling the device.

You can download the latest NI-VISA runtime engine or full version from the NI official website. Their installation steps are basically the same.

Please refer to the following steps to install NI-VISA (the example uses the full version of NI-VISA5.4):


- a. Download the appropriate version of NI-VISA.
- b. Double-click visa540_full.exe, and the dialog box will pop up as follows:

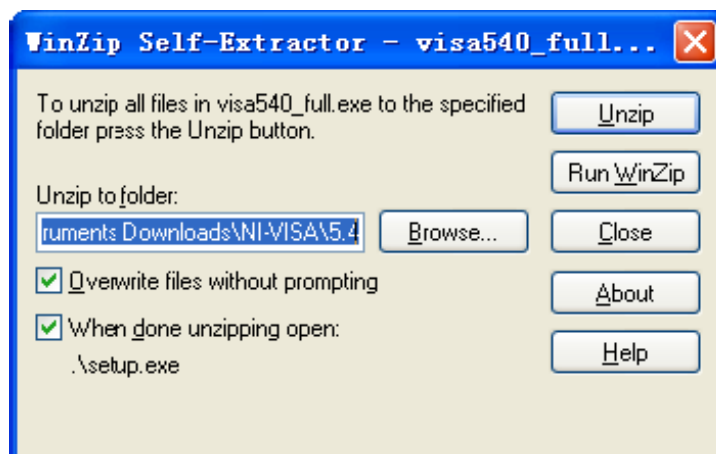


- c. Click Unzip. Then the installation process will launch automatically after unzipping files. If your computer needs to install the .NET Framework 4, it shall auto-start.




- d. The NI-VISA install dialog is shown above. Click Next to start the installation process.

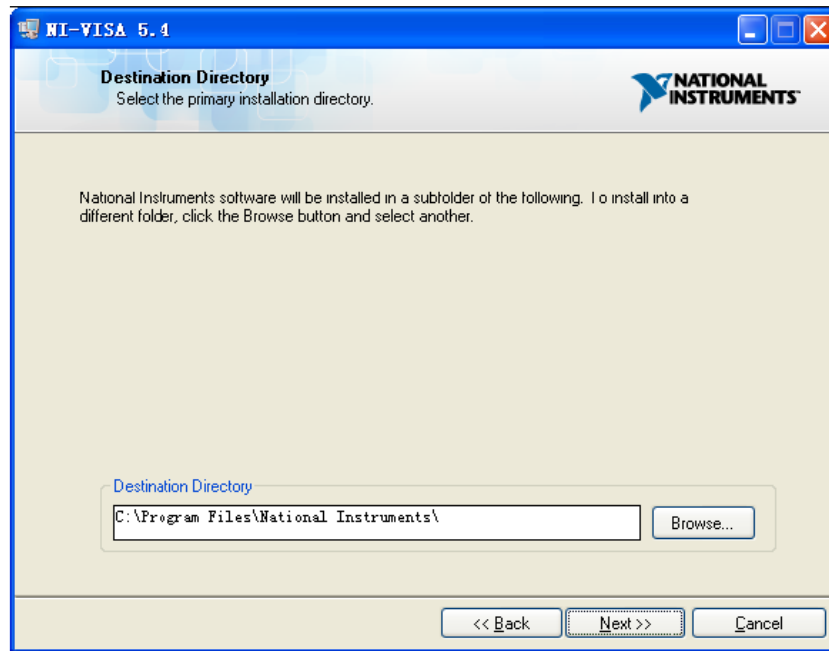


- e. Set the installation path. The default path is “C:\Program Files\National Instruments\”. You can also modify the installation path. Click Next and the dialog box will appear as shown below.

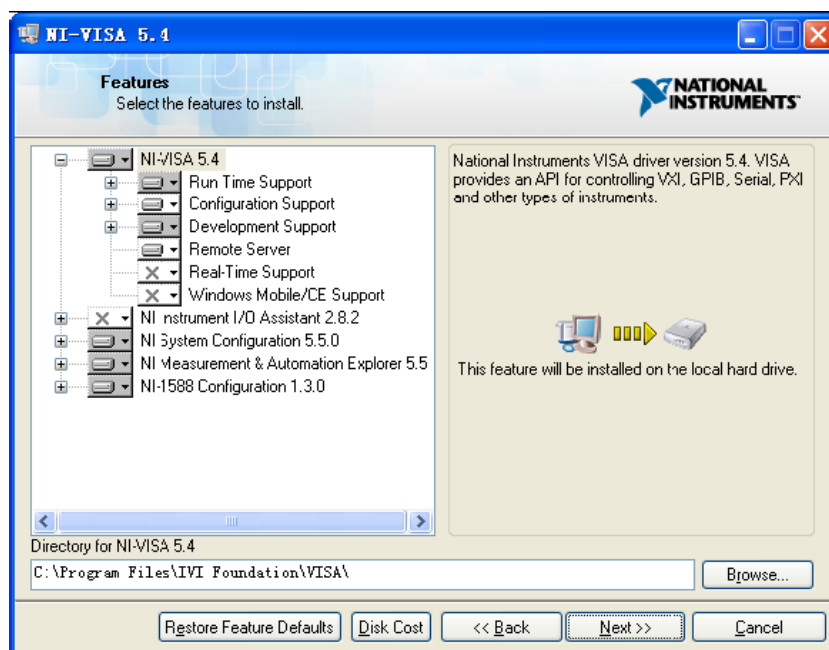

- f. Click Next twice. In the License Agreement dialog, select “I accept the above 2 License Agreement(s).” and click Next. The dialog box will appear as shown below:

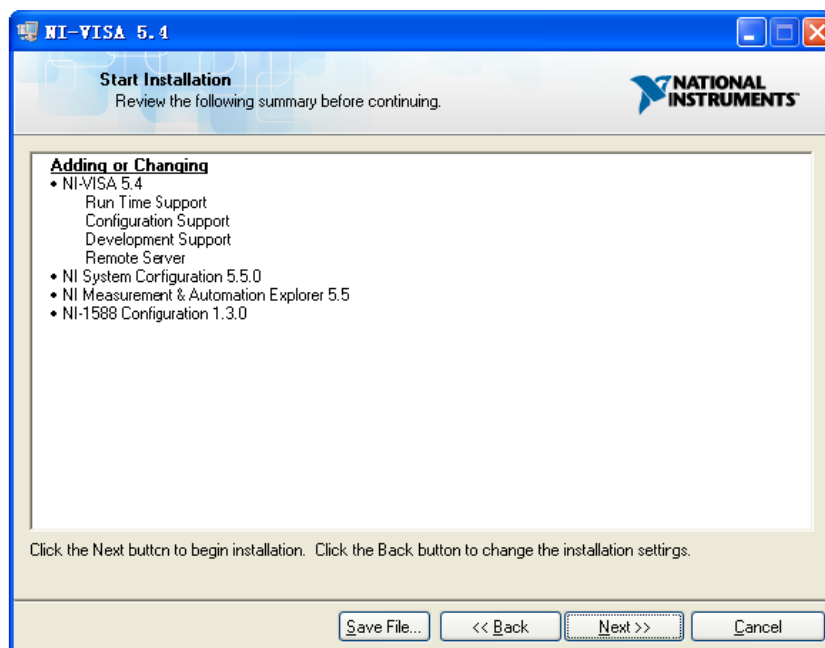

- g. Click Next to begin installation.

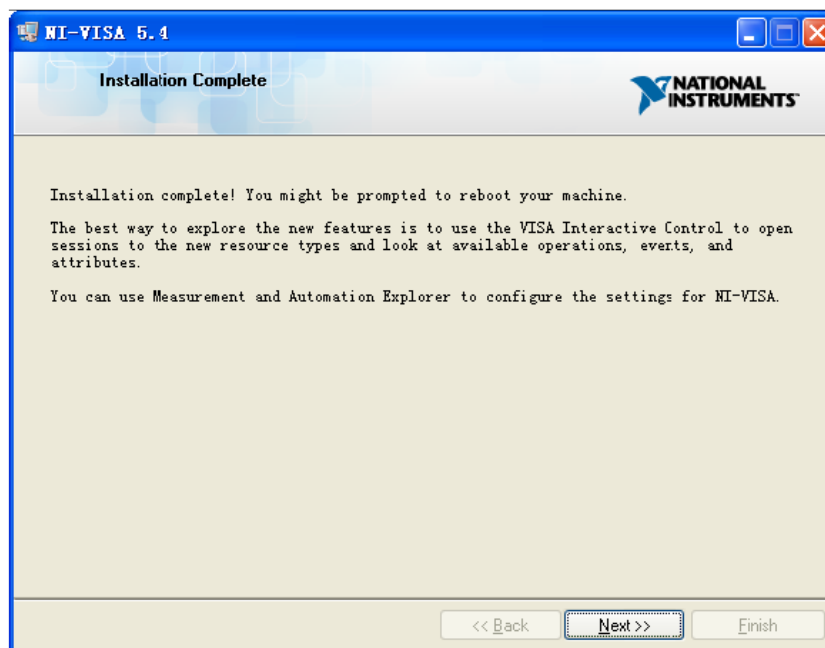

- h. Now the installation is complete. Reboot your computer.

1.1.2 Connect the instrument to computer

The multi-channel microwave signal generator may be able to communicate with the computer through the USB, LAN or USB-GPIB interface.

1.1.2.1 Connect using USB interface

Please refer to the following steps to finish the connection via the USB interface:


1. Install NI-VISA on your computer to obtain the USB-TMC driver.
2. Connect the USB Device interface of the signal generator to the USB Host interface of the computer with a USB A-B cable.
3. Turn on the signal generator.

The signal generator will be automatically detected as a new USB device.

1.1.2.2 Connect using LAN interface

Please refer to the following steps to finish the connection via the LAN interface:

1. Install NI-VISA on your computer to obtain the VXI driver.
2. Use a network cable to connect the signal generator to your computer or the local area network.
3. Turn on the signal generator.
4. Press HOME → Interface to enter the LAN Setting menu.
5. Set the LAN as Static or DHCP:
 - ◆ DHCP: The DHCP server in the current network will automatically assign network parameters (IP address, subnet mask, gateway) to the signal generator.
 - ◆ Static: You can manually set the IP address, subnet mask, and gateway.

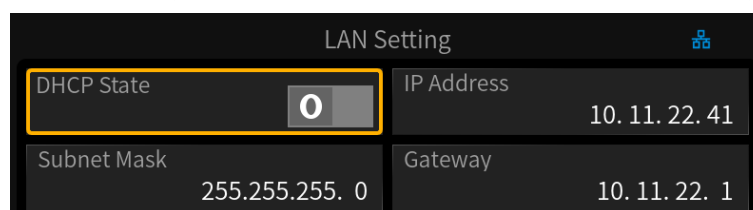

The signal generator will be automatically or manually detected as a new LAN device.

1.1.2.3 Connect using USB Host interface (With USB-GPIB Adaptor)

Please refer to the following steps to finish the connection via the LAN interface:

1. Install the NI-VISA GPIB driver on the computer.
2. Use the SIGLENT USB-GPIB adapter to connect the USB Host interface of the signal generator to the GPIB interface of the computer.



3. Turn on the signal generator.
 4. Press HOME → Interface and enter the GPIB number in GPIB Address.
- The signal generator will be automatically detected as a new GPIB device.

1.2 Remote Control

1.2.1 User-defined Programming

Users can send SCPI commands through the computer to program and control the multi-channel microwave signal generator. For details, please refer to the introduction in the “Programming Examples” chapter.

1.2.2 Send SCPI via NI-MAX

NI-MAX is a program created and maintained by National Instruments. It provides basic remote control interfaces for VXI, LAN, USB, GPIB, and Serial communications. Users can send SCPI commands through NI-MAX to remotely control the signal generator.


The following describes the steps for connecting a device through a USB, LAN, or GPIB interface in NI-MAX and sending SCPI to the device.

1.2.2.1 Using USB

1. Run NI-MAX.
2. Click “Devices and Interfaces” in the upper left corner of the software.
3. Find the USBTMC device symbol: .
4. Select the signal generator device and click the “Open VISA Test Panel” button.




5. Select the “Input/Output” page in the VISA test panel. At this time, you can enter SCPI in the input field to write or query. Click the “Query” button as shown below to query the device’s IDN:

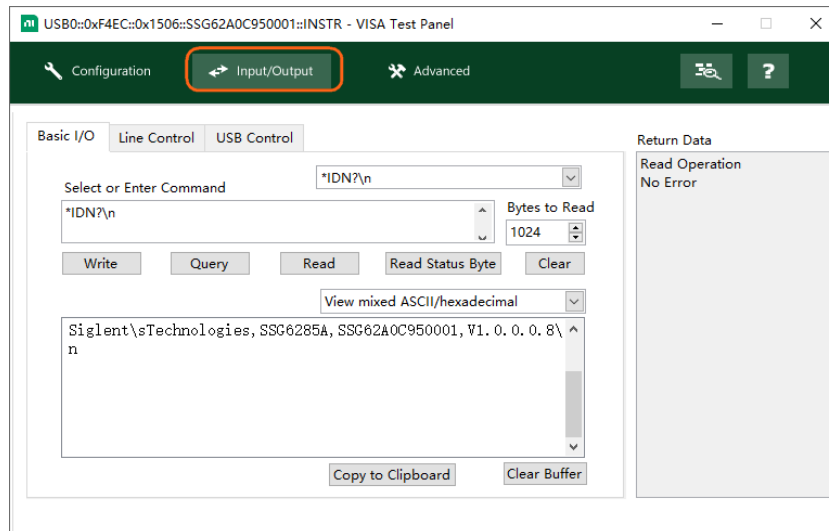


1.2.2.2 Using LAN


1. Run NI-MAX.
2. Click “Devices and Interfaces” > “Network Devices” in the upper left corner of the software.
3. Click “Add Network Device” > “VISA TCP/IP Resource...”.

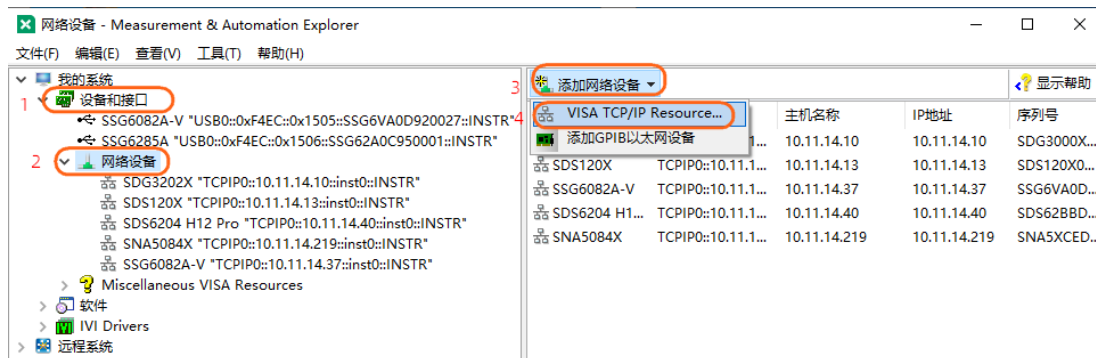


4. In the pop-up “Create New...” window, select “Manual Entry of LAN Instrument” and then click Next.

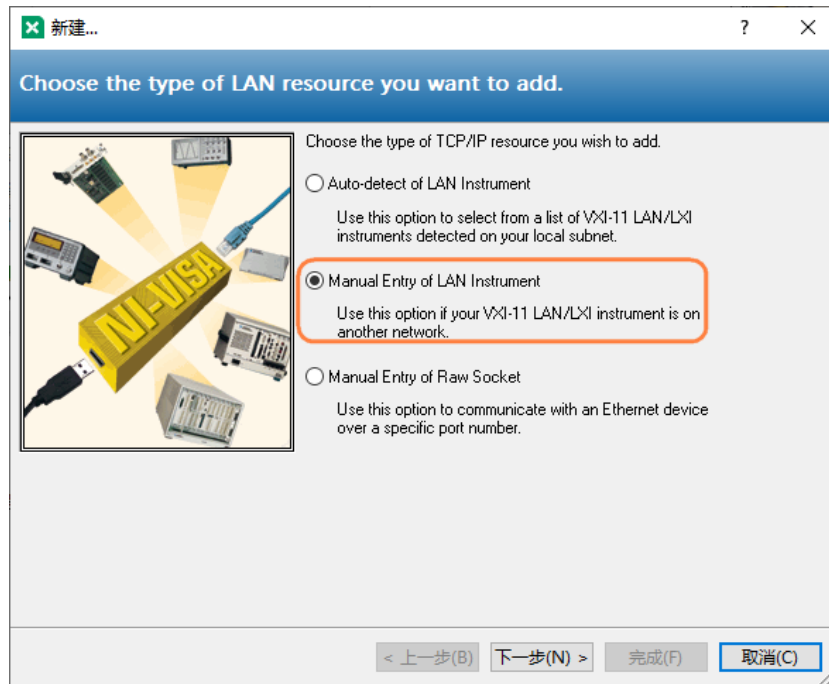


5. Enter the IP address of the signal generator in "Hostname or IP address". You can click "Validate" to verify whether the device can be connected via the entered IP.

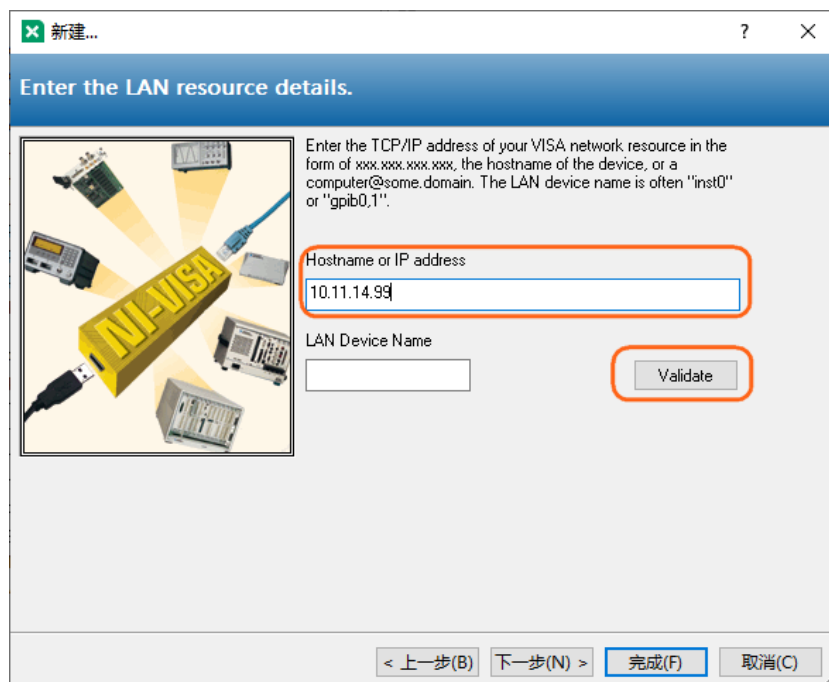

6. Click "Finish" to establish the connection.
7. After a short scan, the resource name of the signal generator should be displayed under "Network Devices".

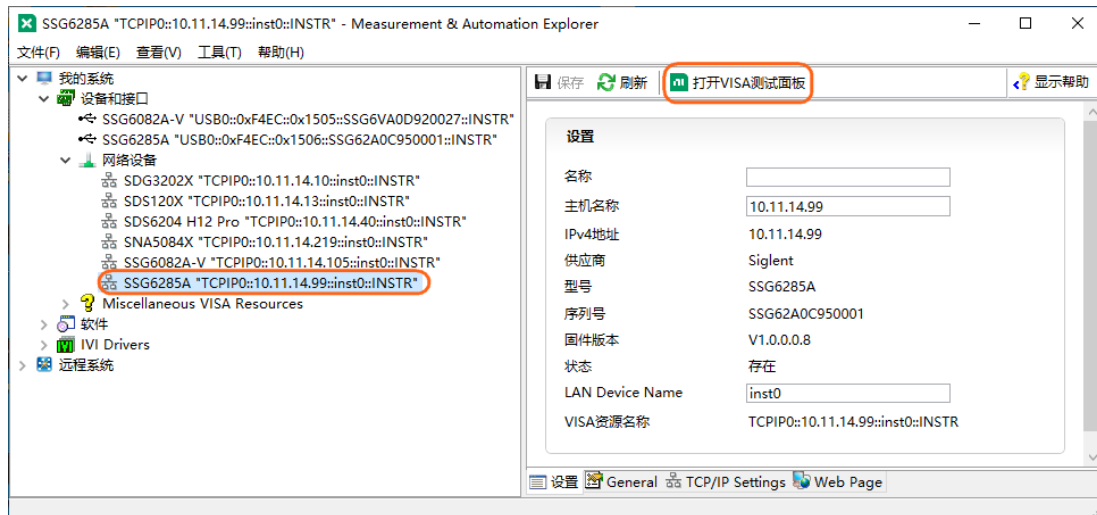

8. Select the signal generator device and click the “Open VISA Test Panel” button.
9. Select the “Input/Output” page in the VISA test panel. At this time, you can enter SCPI in the input field to write or query. Click the “Query” button as shown below to query the device’s IDN:

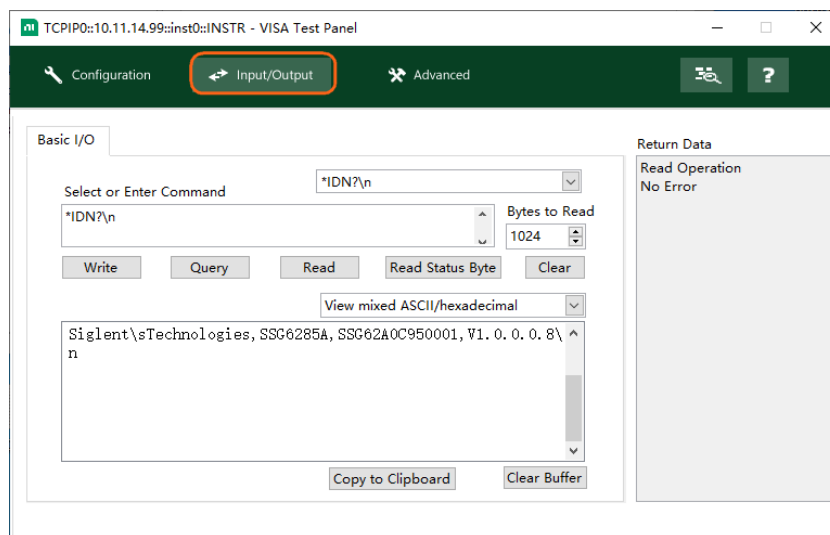


1.2.2.3 Using USB-GPIB


1. Run NI-MAX.
2. Click “Devices and Interfaces” in the upper left corner of the software.
3. Find the “GPIB-USB-HS” device symbol.
4. Select the signal generator device and click the “Open VISA Test Panel” button.



5. Select the “Configuration” > “I/O Settings” in the VISA test panel. Check the Enable Termination Character option, and click Apply Changes button.

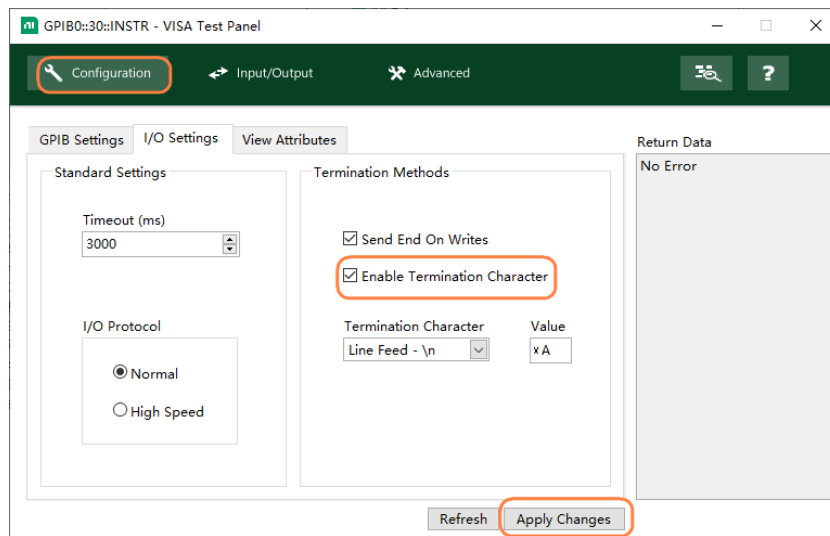

6. Select the “Input/Output” page in the VISA test panel. At this time, you can enter SCPI in the input field to write or query. Click the “Query” button as shown below to query the device’s IDN:

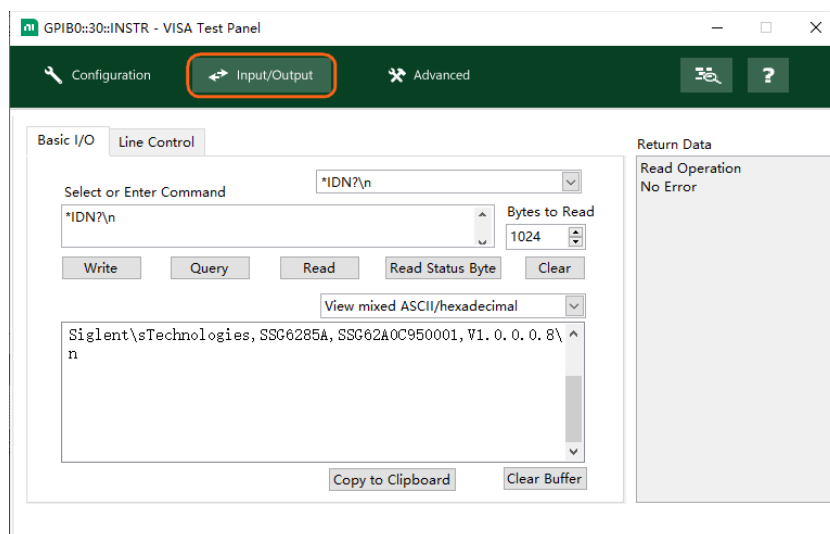

1.2.3 Send SCPI over Telnet


Telnet provides a way to communicate with the signal generator through the LAN interface. The Telnet protocol supports sending SCPI commands from the computer to the signal generator in a manner similar to communicating with the signal generator via USB. Sending and receiving information is interactive, and only one command can be sent at a time. Windows operating systems use a command prompt style interface as a Telnet client.

The steps are as follows:


1. On the computer desktop, click Start, then right-click and select Run. Enter *cmd* in the run window and click OK. The command prompt window opens.



2. In the command prompt window, enter *telnet <ip address> 5024* and press Enter. A Telnet window that can communicate with the instrument will pop up:

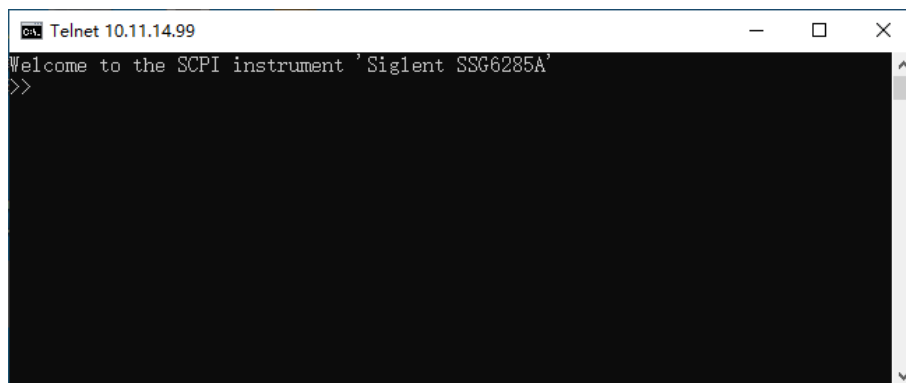


3. After the ">>" prompt, you can enter a SCPI command to remotely control the signal generator. For example, enter **IDN?*, this command will return the company name, machine model, serial number and firmware version number.

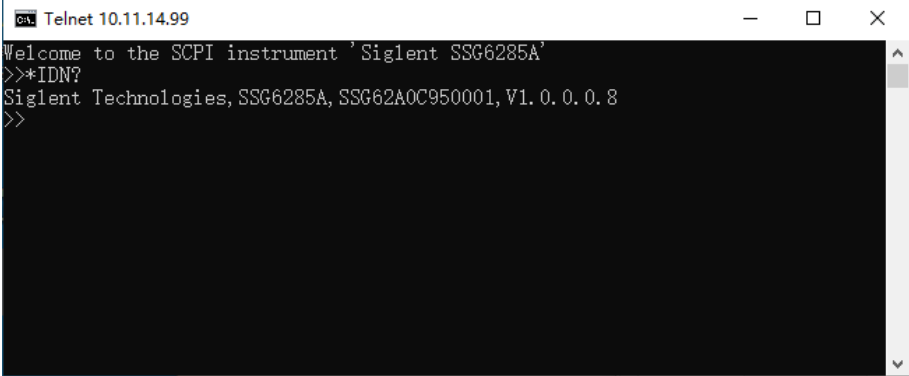


```
ca Telnet 10.11.14.99
Welcome to the SCPI instrument 'Siglent SSG6285A'
>>*IDN?
Siglent Technologies, SSG6285A, SSG62A0C950001, V1.0.0.0.8
>>
```

4. Press Ctrl+] keys simultaneously to exit the SCPI session with the instrument.

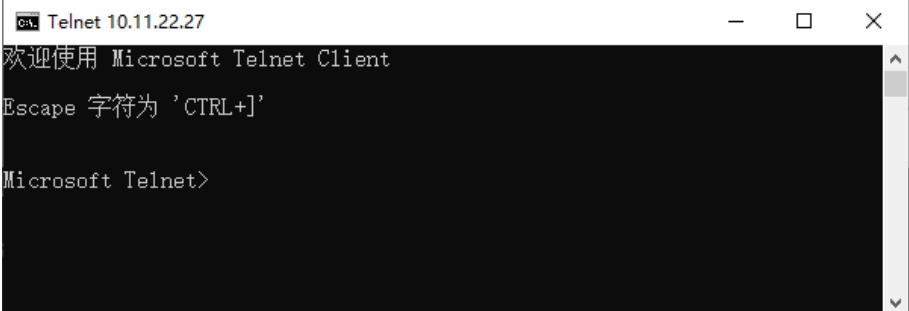


```
ca Telnet 10.11.22.27
欢迎使用 Microsoft Telnet Client
Escape 字符为 'CTRL+]'
Microsoft Telnet>
```

5. To re-enter the SCPI session with the instrument, you can enter *open <ip Address> 5024* and press Enter.

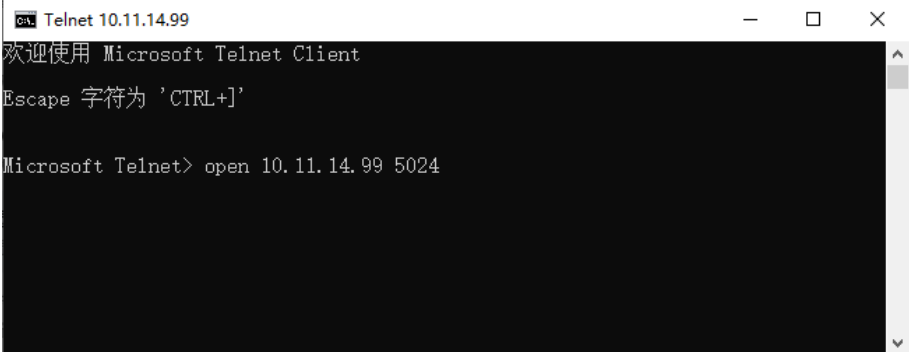

```
ca Telnet 10.11.14.99
欢迎使用 Microsoft Telnet Client
Escape 字符为 'CTRL+]'
Microsoft Telnet> open 10.11.14.99 5024
```

6. To close the Telnet window, type *Quit* and press Enter.

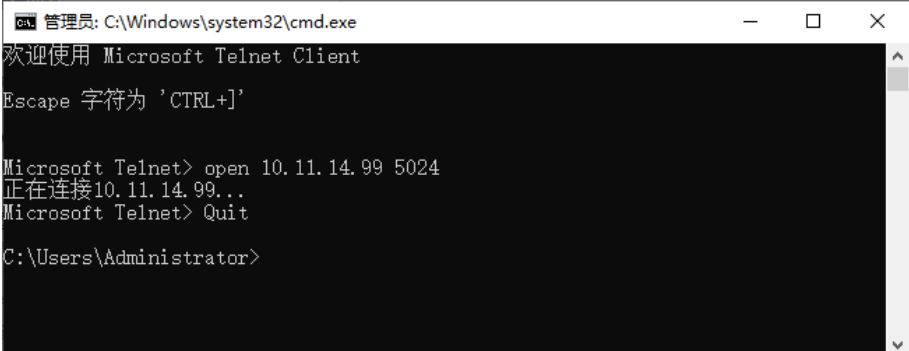

```
ca 管理员: C:\Windows\system32\cmd.exe
欢迎使用 Microsoft Telnet Client
Escape 字符为 'CTRL+]'
Microsoft Telnet> open 10.11.14.99 5024
正在连接10.11.14.99...
Microsoft Telnet> Quit
C:\Users\Administrator>
```

1.2.4 Send SCPI over Socket

Socket API can be used to control the signal generator through the LAN interface without installing any other libraries, which can reduce the complexity of programming.

For detailed information, please refer to the “Socket Examples” chapter of “Programming Examples”.

SOCKET ADDRESS	IP address + port number
IP ADDRESS	SSG IP address
PORT NUMBER	5025

2 Introduction to the SCPI Language

2.1 Command Format

SCPI commands are tree-like hierarchical structures, including multiple subsystems. Each subsystem consists of a root keyword and one or several hierarchical keywords. The command line usually starts with a colon ":" and keywords are separated by a colon ":". The keyword is followed by optional parameter settings. The command and parameters are separated by "space". For multiple parameters, the parameters are separated by commas ",". Add a question mark "?" after the command line to indicate querying this function.

For example:

```
:SOURce:FREQuency <freq>
```

```
:SOURce:FREQuency?
```

SOURce is the root keyword of the command, and FREQuency is the second-level keyword. The command line starts with a colon ":", and colons separate keywords at each level. <freq> represents a settable parameter. The command: SOURce:FREQuency and the parameter <freq> are separated by a "space". The question mark "?" indicates query, and the instrument will return a response string after receiving the query command.

2.2 Symbol Instruction

The following are the symbols used in the SCPI commands:

1. Angular brackets < >

The contents in angular brackets < > are command parameters and must be replaced with a valid value. For example:

POWer:SPC:TARGet <power> command, you can send as POWer:SPC:TARGet 0.

2. Square brackets []

Contents in square brackets (command keywords or default parameters) can be omitted. If you omit the keyword in square brackets, the command still produces the same effect. If a default parameter in square brackets is omitted, the default parameter still takes effect.

3. Vertical lines |

Vertical bars are used to separate multiple enumeration values, one of which must be selected when sending a command. For example:

In the [:SOURce<ch>]:AM:STATe OFF|ON|0|1 command, the optional command parameters are "OFF", "ON", "0" or "1".

4. Braces {}

Parameters in braces are optional and may not be set, or may be set once or multiple times. For example:

In the :CALCulate:LLINe[1]|2:DATA <x-axis>,<ampl>{<x-axis>,<ampl>} command, {<x-axis>,<ampl>} in braces can be omitted, or one or more pairs of frequency and amplitude parameters can be set.

2.3 Parameter Type

The parameters in the commands introduced in this manual include 6 types: Boolean, enumeration, integer, float, string and discrete.

1. Boolean

The parameter in the command could be "OFF", "ON", "0" or "1".

For example:

```
[[:SOURce<ch>]:FM:STATe OFF|ON|0|1
```

2. Enumeration

Parameter should be one of the listed values.

For example:

In [:SOURce<ch>]:SWEep:STATe OFF|FREQuency|LEVel|LEV_FREQ command, valid parameters are "OFF", "FREQuency", "LEVel" or "LEV_FREQ".

3. Integer

Unless otherwise stated, the parameter can be any integer within the valid value range.

For example:

In [:SOURce<ch>]:SWEep:STEP:POINts <value> command, the parameter <value> can be set to any integer between 2 and 65535.

4. Float

Parameters can take any value within the valid range according to accuracy requirements (usually the default accuracy is nine decimal places).

For example:

In [:SOURce<ch>]:POWer:OFFSet <value> command, the parameter <value> can be set to any real number between -100 and 100.

5. String

The parameter should be the combination of ASCII characters.

For example:

In :SYSTem:COMMunicate:LAN:IPADdress <"xxx.xxx.xxx.xxx"> command, the IP address can be set as the string "192.168.1.12".

6. Discrete

The parameter could only be one of the specified values and these values are discontinuous.

For example:

In [:SENSe]:BWIDth:VIDeo:RATio <number> command, the parameter <number> could only be one of 0.001, 0.003, 0.01, 0.03, 0.1, 0.3, 1.0, 3.0, 10.0, 30.0, 100.0, 300.0, 1000.0.

2.4 Command Abbreviation

All SCPI commands are case-insensitive. You can enter the complete command in all uppercase or all lowercase. You can also use abbreviations, in which case the abbreviated command must contain all uppercase letters in the command format.

For example:

:CORRection:FLATness:COUNt?

You can send in any of the following writing methods:

:CORRection:FLATness:COUNt?

:CORRECTION:FLATNESS:COUNT?

:correction:flatness:count?

You can also abbreviate it to:

:CORR:FLAT:COUN?

3 Commands

3.1 IEEE 488.2 Common Commands

The IEEE standards defined the common commands used for querying the basic information of the instrument and performing basic operations. These commands usually start with "*" and the length of the command keyword is usually 3 characters.

3.1.1 Identification Query (*IDN?)

SYNTAX	*IDN?
DESCRIPTION	This command reads the product information (manufacturer, device model, serial number, and firmware revision number) of the device.
EQUIVALENT MENU	None
EXAMPLE	<i>*IDN?</i> Return: <i>Siglent Technologies,SSG6285A,SSG62A0C950001,V1.0.0.0.8\n</i>

3.1.2 Reset (*RST)

SYNTAX	*RST
DESCRIPTION	Restore the device state to its initial state.
EQUIVALENT MENU	None
EXAMPLE	<i>*RST</i>

3.1.3 Clear Status (*CLS)

SYNTAX	*CLS
DESCRIPTION	Clear the values of all status event registers and clear the error queue.
EQUIVALENT MENU	None
EXAMPLE	<i>*CLS</i>

3.1.4 Standard Event Status Enable (*ESE)

SYNTAX	*ESE <number> *ESE?
DESCRIPTION	This command sets/gets the value of the Standard Event Status Enable Register.
DATA TYPE	Integer
RANGE	0 to 255
EQUIVALENT MENU	None
EXAMPLE	<i>*ESE 16</i> <i>*ESE?</i> Return: <i>16ln</i>

3.1.5 Standard Event Status Register Query (*ESR?)

SYNTAX	*ESR?
DESCRIPTION	This command reads the value of the Standard Event Status Register. Execution of this command clears the register value.
EQUIVALENT MENU	None
EXAMPLE	<i>*ESR?</i> Return: <i>0ln</i>

3.1.6 Operation Complete Query (*OPC)

SYNTAX	*OPC *OPC?
DESCRIPTION	This command sets/gets 1 the OPC bit (bit 0) of the Standard Event Status Register when all of pending operations complete.
EQUIVALENT MENU	None
EXAMPLE	<i>*OPC</i> <i>*OPC?</i> Return: <i>1ln</i>

3.1.7 Service Request Enable (*SRE)

SYNTAX	*SRE <integer> *SRE?
DESCRIPTION	This command sets/gets the value of Service Request Enable Register.
DATA TYPE	Integer
RANGE	0 to 255
EQUIVALENT MENU	None
EXAMPLE	<i>*SRE 24</i> <i>*SRE?</i> Return: <i>24\n</i>

3.1.8 Status Byte Query (*STB?)

SYNTAX	*STB?
DESCRIPTION	This command reads the value of Status Byte Register.
EQUIVALENT MENU	None
EXAMPLE	<i>*STB?</i> Return: <i>72\n</i>

3.1.9 Wait-to-Continue (*WAI)

SYNTAX	*WAI
DESCRIPTION	This command waits for the execution of all objects sent before this command to be completed.
EQUIVALENT MENU	None
EXAMPLE	<i>*WAI</i>

3.1.10 Self Test Query (*TST?)

SYNTAX	*TST?
DESCRIPTION	This command queries the instrument self-test results..
EQUIVALENT MENU	None
EXAMPLE	<i>*TST?</i> Return: <i>0ln</i>

3.2 SYSTem Commands

3.2.1 System Configuration

3.2.1.1 System Time (:SYSTem:TIME)

SYNTAX	:SYSTem:TIME <hhmmss> :SYSTem:TIME?
DESCRIPTION	This command sets/gets the system time.
DATA TYPE	String
RANGE	Hours(0 ~ 23), minutes(0 ~ 59), seconds(0 ~ 59)
RETURN	String
EQUIVALENT MENU	 >  >  > Setting > Time Setting
EXAMPLE	<i>:SYSTem:TIME 182559</i> <i>:SYSTem:TIME?</i> Return: <i>182613\n</i>

3.2.1.2 System Date (:SYSTem:DATE)

SYNTAX	:SYSTem:DATE <yyyymmdd> :SYSTem:DATE?
DESCRIPTION	This command sets/gets the system date.
DATA TYPE	String
RANGE	Years(four digits), month(1 ~ 12), date(1 ~ 31)
RETURN	String
EQUIVALENT MENU	 >  >  > Setting > Time Setting
EXAMPLE	<i>:SYSTem:DATE 20050101</i> <i>:SYSTem:DATE?</i> Return: <i>20050101\n</i>

3.2.1.3 IP Address (:SYSTem:COMMunicate:LAN:IPADdress)

SYNTAX	:SYSTem:COMMunicate:LAN:IPADdress <“xxx.xxx.xxx.xxx”> :SYSTem:COMMunicate:LAN:IPADdress?
--------	---

DESCRIPTION	This command sets/gets the IP address of the device when the IP assignment is set to Static.
DATA TYPE	String
RANGE	Conforms to the IP address standard (0-255:0-255:0-255)
RETURN	String
EQUIVALENT MENU	 >  >  > Interface > LAN Setting > IP Address
EXAMPLE	<pre><i>:SYSTem:COMMUnicate:LAN:IPADdress "192.168.1.12"</i> :SYSTem:COMMUnicate:LAN:IPADdress?</pre> Return: <pre><i>"192.168.1.12"ln</i></pre>

3.2.1.4 Gateway (:SYSTem:COMMUnicate:LAN:GATeway)

SYNTAX	<pre>:SYSTem:COMMUnicate:LAN:GATeway <"xxx.xxx.xxx.xxx"> :SYSTem:COMMUnicate:LAN:GATeway?</pre>
DESCRIPTION	This command sets/gets the gateway of the device when the IP assignment is set to Static.
DATA TYPE	String
RANGE	Conforms to the IP address standard (0-255:0-255:0-255)
RETURN	String
EQUIVALENT MENU	 >  >  > Interface > LAN Setting > Gateway
EXAMPLE	<pre><i>:SYSTem:COMMUnicate:LAN:GATeway "192.168.1.1"</i> :SYSTem:COMMUnicate:LAN:GATeway?</pre> Return: <pre><i>"192.168.1.1"ln</i></pre>

3.2.1.5 Subnet Mask (:SYSTem:COMMUnicate:LAN:SMASK)

SYNTAX	<pre>:SYSTem:COMMUnicate:LAN:SMASK <"xxx.xxx.xxx.xxx"> :SYSTem:COMMUnicate:LAN:SMASK?</pre>
DESCRIPTION	This command sets/gets the subnet mask of the device when the IP assignment is set to Static.
DATA TYPE	String
RANGE	Conforms to the IP address standard (0-255:0-255:0-255)

RETURN	String
EQUIVALENT MENU	 >  >  > Interface > LAN Setting > Subnet Mask
EXAMPLE	<pre> :SYSTem:COMMUnicate:LAN:SMASk "255.255.255.0" :SYSTem:COMMUnicate:LAN:SMASk? </pre> Return: <pre> "255.255.255.0"ln </pre>

3.2.1.6 IP Config (:SYSTem:COMMUnicate:LAN:TYPE)

SYNTAX	<pre> :SYSTem:COMMUnicate:LAN:TYPE STATICIDHCP :SYSTem:COMMUnicate:LAN:TYPE? </pre>
DESCRIPTION	This command sets/gets IP assignment type.
DATA TYPE	Enumeration
RANGE	STATICIDHCP
RETURN	Enumeration
EQUIVALENT MENU	 >  >  > Interface > LAN Setting > DHCP State
EXAMPLE	<pre> :SYSTem:COMMUnicate:LAN:TYPE STATIC :SYSTem:COMMUnicate:LAN:TYPE? </pre> Return: <pre> STATICln </pre>

3.2.1.7 Language (SYSTem:LANGUage)

SYNTAX	<pre> :SYSTem:LANGUage CHINese ENGLish :SYSTem:LANGUage? </pre>
DESCRIPTION	This command sets/gets the system language.
DATA TYPE	Enumeration
RANGE	CHINese ENGLish
RETURN	Enumeration
EQUIVALENT MENU	 >  >  > Setting > Language
EXAMPLE	<pre> :SYSTem:LANGUage CHINese :SYSTem:LANGUage? </pre> Return: <pre> CHINeseIn </pre>

3.2.1.8 Screen Saver (SYSTem:SCReen:SAVer)

SYNTAX	:SYSTem:SCReen:SAVer OFF 10S 1MIN 5MIN 15MIN 30MIN 1HOUR 2HOUR :SYSTem:SCReen:SAVer?
DESCRIPTION	This command sets/gets the type of system screen saver.
DATA TYPE	Enumeration
RANGE	OFF 10S 1MIN 5MIN 15MIN 30MIN 1HOUR 2HOUR
RETURN	Enumeration
DEFAULT VALUE	OFF
EQUIVALENT MENU	 >  >  > Setting > Screen Saver
EXAMPLE	<i>:SYSTem:SCReen:SAVer 30MIN</i> <i>:SYSTem:SCReen:SAVer?</i> Return: <i>30MIN\n</i>

3.2.1.9 Beeper (SYSTem:ALARm)

SYNTAX	:SYSTem:ALARm ON OFF 1 0 :SYSTem:ALARm?
DESCRIPTION	This command sets/gets the state of system beeper.
DATA TYPE	Boolean
RANGE	ON OFF 1 0
RETURN	1 0
DEFAULT VALUE	0
EQUIVALENT MENU	 >  >  > Setting > Beeper
EXAMPLE	<i>:SYSTem:ALARm ON</i> <i>:SYSTem:ALARm?</i> Return: <i>1\n</i>

3.2.1.10 Setup Type (:SYSTem:PON:TYPE)

SYNTAX	:SYSTem:PON:TYPE DFT LAST :SYSTem:PON:TYPE?
--------	--

DESCRIPTION	This command sets/gets the system startup type.
DATA TYPE	Enumeration
RANGE	DFT LAST
RETURN	Enumeration
DEFAULT VALUE	None
EQUIVALENT MENU	 >  >  > Setting > Setup Type
EXAMPLE	<pre> :SYSTem:PON:TYPE LAST :SYSTem:PON:TYPE? Return: LASTln </pre>

3.2.1.11 Power On Line (SYSTem:POWeron:TYPE)

SYNTAX	<pre> :SYSTem:POWeron:TYPE ON OFF 1 0 :SYSTem:POWeron:TYPE? </pre>
DESCRIPTION	This command sets/gets whether the system is powered on or not.
DATA TYPE	Boolean
RANGE	ON OFF 1 0
RETURN	1 0
DEFAULT VALUE	0
EQUIVALENT MENU	 >  >  > Setting > Power On Line
EXAMPLE	<pre> :SYSTem:POWeron:TYPE ON :SYSTem:POWeron:TYPE? Return: 1ln </pre>

3.2.1.12 10M Adjustment State (:SYSTem:REF:DAC:STAT)

SYNTAX	<pre> :SYSTem:REF:DAC:STAT ON OFF 1 0 :SYSTem:REF:DAC:STAT? </pre>
DESCRIPTION	This command sets/gets the state of system 10M adjustment.
DATA TYPE	Boolean
RANGE	ON OFF 1 0

RETURN	1 0
DEFAULT VALUE	0
EQUIVALENT MENU	 >  >  > Setting > 10M Adjustment
EXAMPLE	<i>:SYSTem:REF:DAC:STAT ON</i> <i>:SYSTem:REF:DAC:STAT?</i> Return: <i>1 n</i>

3.2.1.13 Ref Osc Code (:SYSTem:REF:DAC)

SYNTAX	:SYSTem:REF:DAC <value> :SYSTem:REF:DAC?
DESCRIPTION	This command sets/gets the system reference oscillator code.
DATA TYPE	Integer
RANGE	0 to 65535
RETURN	Integer
DEFAULT VALUE	None
EQUIVALENT MENU	 >  >  > Setting > 10M Adjustment > Ref Osc Code
EXAMPLE	<i>:SYSTem:REF:DAC 43000</i> <i>:SYSTem:REF:DAC?</i> Return: <i>43000 n</i>

3.2.1.14 Ref Osc Code Store (:SYSTem:REF:DAC:SAVE)

SYNTAX	:SYSTem:REF:DAC:SAVE <"file_name">
DESCRIPTION	This command saves the system's reference oscillator code into the file.
DATA TYPE	String
RANGE	None
EQUIVALENT MENU	 >  >  > Setting > 10M Adjustment > Save Ref Osc Setting
EXAMPLE	<i>:SYSTem:REF:DAC:SAVE "U-disk3/test.dac"</i>

3.2.1.15 Ref Osc Code Load (:SYSTem:REF:DAC:LOAD)

SYNTAX	:SYSTem:REF:DAC:LOAD <"file_name">
DESCRIPTION	This command loads the reference oscillator code from the file.
DATA TYPE	String
RANGE	None
EQUIVALENT MENU	 >  >  > Setting > 10M Adjustment > Recall Ref Osc Setting
EXAMPLE	<i>:SYSTem:REF:DAC:LOAD "U-disk3/test.dac"</i>

3.2.1.16 Reset Ref Osc Code to Default (:SYSTem:REF:DAC:DEFault)

SYNTAX	:SYSTem:REF:DAC:DEFault
DESCRIPTION	This command resets the reference oscillator code to default value.
EQUIVALENT MENU	 >  >  > Setting > 10M Adjustment > Reset to Default
EXAMPLE	<i>:SYSTem:REF:DAC:DEFault</i>

3.2.1.17 GPIB Address (SYSTem:GPIB)

SYNTAX	:SYSTem:GPIB <value> :SYSTem:GPIB?
DESCRIPTION	This command sets/gets the GPIB address of the device.
DATA TYPE	Integer
RANGE	1 to 30
RETURN	Integer
DEFAULT VALUE	18
EQUIVALENT MENU	 >  >  > Interface > GPIB Address
EXAMPLE	<i>:SYSTem:GPIB 10</i> <i>:SYSTem:GPIB?</i> Return: <i>10\n</i>

3.2.1.18 Quit Remote Control State (SYSTem:REMOte 0)

SYNTAX	:SYSTem:REMOte 0
DESCRIPTION	Send this command to exit the remote mode of the system.
EQUIVALENT MENU	ESC
EXAMPLE	<i>:SYSTem:REMOte 0</i>

3.2.1.19 Query Clock Reference Source (:SYSTem:CLOCK?)

SYNTAX	:SYSTem:CLOCK?
DESCRIPTION	Query whether the clock reference source used by the instrument is internal or external.
RETURN	EXTERNAL: The instrument uses an external clock reference, INTERNAL: The instrument uses an internal clock reference.
EQUIVALENT MENU	EXTERNAL: HOME > EXT REF logo, INTERNAL: No logo.
EXAMPLE	<i>:SYSTem:CLOCK?</i> Return: <i>EXTERNAL In</i>

3.2.2 System Reset/Preset

3.2.2.1 System Preset (:SYSTem:PRESet)

SYNTAX	:SYSTem:PRESet
DESCRIPTION	This command presets the status of the instrument based on the preset type.
EQUIVALENT MENU	HOME >  >  > Preset, or PRESET
EXAMPLE	Reset the instrument to its default configuration: <pre><i>:SYSTem:PRESet:TYPE DFT</i></pre> <pre><i>:SYSTem:PRESet</i></pre> Reset the instrument to its current configuration: <pre><i>:SYSTem:PRESet:TYPE USER</i></pre> <pre><i>:SYSTem:PRESet:SAVE</i></pre> <pre><i>:SYSTem:PRESet</i></pre> Reset the instrument to the configuration in the file: <pre><i>:SYSTem:PRESet:TYPE USER</i></pre> <pre><i>:SYSTem:PRESet:PATH "Local/test.xml"</i></pre> <pre><i>:SYSTem:PRESet</i></pre>

3.2.2.2 Preset Save (:SYSTem:PRESet:SAVE)

SYNTAX	:SYSTem:PRESet:SAVE
DESCRIPTION	This command saves the current system configuration.
EQUIVALENT MENU	None
EXAMPLE	Reset the instrument to its current configuration: <pre><i>:SYSTem:PRESet:TYPE USER</i></pre> <pre><i>:SYSTem:PRESet:SAVE</i></pre> <pre><i>:SYSTem:PRESet</i></pre>

3.2.2.3 Preset Path (:SYSTem:PRESet:PATH)

SYNTAX	:SYSTem:PRESet:PATH <"file_name">
DESCRIPTION	This command saves the current system configuration into a file.
DATA TYPE	String
RANGE	None

EQUIVALENT MENU  >  >  > Setting > Preset Type (User) > Save

EXAMPLE *:SYSTem:PRESet:PATH "Local/test.xml"*
:SYSTem:PRESet:PATH "U-disk1/test.xml"

3.2.2.4 Preset Type (:SYSTem:PRESet:TYPE)

SYNTAX :SYSTem:PRESet:TYPE DFT|USER
:SYSTem:PRESet:TYPE?

DESCRIPTION This command sets/gets the preset type of the system.

DATA TYPE Enumeration

RANGE DFT|USER

RETURN Enumeration

DEFAULT VALUE DFT

EQUIVALENT MENU  >  >  > Setting > Preset Type

EXAMPLE *:SYSTem:PRESet:TYPE DFT*
:SYSTem:PRESet:TYPE?
Return:
DFT\n

3.2.2.5 Factory Reset (:SYSTem:FDEFault)

SYNTAX :SYSTem:FDEFault

DESCRIPTION This command restores the instrument status to factory settings.

EQUIVALENT MENU  >  >  > Setting > Factory Reset

EXAMPLE *:SYSTem:FDEFault*

3.2.2.6 Reset & Clear (SYSTem:RESet:CLEAr)

SYNTAX :SYSTem:RESet:CLEAr

DESCRIPTION Restore the instrument status to factory settings and clear the user files in the Local folder.

EQUIVALENT MENU  >  >  > Setting > Reset & Clear

EXAMPLE *:SYSTem:RESet:CLEAr*

3.3 OUTPut Commands

3.3.1 RF Output ([:SOURce<ch>]:OUTPut)

SYNTAX	[:SOURce<ch>]:OUTPutON OFF 1 0
DESCRIPTION	This command sets/gets the output status of the specified channel .
DATA TYPE	Boolean
RANGE	ON OFF 1 0
RETURN	1 0
DEFAULT VALUE	0
EQUIVALENT SCPI	[:SOURce<ch>]:OUTPut ON OFF 1 0
EQUIVALENT MENU	RF ON/OFF
EXAMPLE	<pre> :SOURce1:OUTPut ON :SOURce1:OUTPut? Return: 1\rn </pre>

3.3.2 Analog Modulation State (:OUTPut:MODulation[:STATe])

SYNTAX	[:SOURce<ch>]:OUTPut:MODulation[:STATe] ON OFF 1 0 [:SOURce<ch>]:OUTPut:MODulation[:STATe]?
DESCRIPTION	This command sets/gets the switch status of analog modulation of the specified channel.
DATA TYPE	Boolean
RANGE	ON OFF 1 0
RETURN	1 0
DEFAULT VALUE	0
EQUIVALENT SCPI	:MODulation ON OFF 1 0 :MODulation?
EQUIVALENT MENU	Analog Mod > On
EXAMPLE	<pre> :SOURce1:OUTPut:MODulation ON :SOURce1:OUTPut:MODulation? Return: 1\rn </pre>

3.4 SOURce Commands

3.4.1 RF Output ([[:SOURce<ch>]:OUTPut])

SYNTAX	[[:SOURce<ch>]:OUTPut ON OFF 1 0]
DESCRIPTION	This command sets the RF output status of the specified channel.
DATA TYPE	Boolean
RANGE	ON OFF 1 0
EQUIVALENT SCPI	:OUTPut[:STATe] ON OFF 1 0
EQUIVALENT MENU	RF ON/OFF
EXAMPLE	<i>:SOURce1:OUTPut ON</i>

3.4.2 Software Trigger([[:SOURce<ch>]:*TRG])

SYNTAX	[[:SOURce<ch>]:*TRG]
DESCRIPTION	When the trigger source is Bus, execute software trigger of the specified channel. Note: the trigger functions involved include sweep trigger, point sweep trigger, LF sweep trigger and pulse modulation trigger, etc.
EQUIVALENT MENU	None
EXAMPLE	<i>:SOURce1:*TRG</i>

3.4.3 Frequency

3.4.3.1 Frequency Display ([[:SOURce<ch>]:FREQuency:DISPlay])

SYNTAX	[[:SOURce<ch>]:FREQuency:DISPlay <freq> [:SOURce<ch>]:FREQuency:DISPlay?]
DESCRIPTION	This command sets/gets the frequency display value of the specified channel in the parameter bar at the top of the screen.
DATA TYPE	Float, unit: Hz, kHz, MHz or GHz, default is Hz
RANGE	Frequency offset + Full frequency range
RETURN	Float, unit: Hz

DEFAULT VALUE	Maximum frequency
EQUIVALENT MENU	Freq
EXAMPLE	<i>:SOURce1:FREQuency:DISPlay 2 MHz</i> <i>:SOURce1:FREQuency:DISPlay?</i> Return: <i>2000000\n</i>

3.4.3.2 Frequency ([[:SOURce<ch>]:FREQuency)

SYNTAX	<i>[[:SOURce<ch>]:FREQuency <freq></i> <i>[[:SOURce<ch>]:FREQuency?</i>
DESCRIPTION	This command sets/gets the frequency of the RF output signal of the specified channel.
DATA TYPE	Float, unit: Hz, kHz, MHz or GHz, default is Hz
RANGE	Full frequency range
RETURN	Float, unit: Hz
DEFAULT VALUE	Maximum frequency
EQUIVALENT MENU	FREQ > Frequency
EXAMPLE	<i>:SOURce1:FREQuency 2 MHz</i> <i>:SOURce1:FREQuency?</i> Return: <i>2000000\n</i>

3.4.3.3 Frequency Offset ([[:SOURce<ch>]:FREQuency:OFFSet)

SYNTAX	<i>[[:SOURce<ch>]:FREQuency:OFFSet <freq></i> <i>[[:SOURce<ch>]:FREQuency:OFFSet?</i>
DESCRIPTION	This command sets/gets the frequency offset of the RF output signal of the specified channel.
DATA TYPE	Float, unit: Hz, kHz, MHz or GHz, default is Hz
RANGE	-200 GHz to 200 GHz
RETURN	Float, unit: Hz
DEFAULT VALUE	0
EQUIVALENT MENU	FREQ > Freq Offset
EXAMPLE	<i>:SOURce1:FREQuency:OFFSet -2 MHz</i>

```
:SOURce1:FREQuency:OFFSet?
```

```
Return:
```

```
-2000000\n
```

3.4.3.4 Phase Offset ([:SOURce<ch>]:PHASe)

SYNTAX	<code>[:SOURce<ch>]:PHASe <phase></code> <code>[:SOURce<ch>]:PHASe?</code>
DESCRIPTION	This command sets/gets the phase offset of the RF signal of the specified channel.
DATA TYPE	Float, unit: degree
RANGE	-360 to 360
RETURN	Float, unit: degree
DEFAULT VALUE	0
EQUIVALENT MENU	FREQ > Phase Offset
EXAMPLE	<pre><i>:SOURce1:PHASe 20</i></pre> <pre><i>:SOURce1:PHASe?</i></pre> <pre>Return:</pre> <pre><i>20\n</i></pre>

3.4.3.5 Reset Phase ([:SOURce<ch>]:PHASe:RESet)

SYNTAX	<code>[:SOURce<ch>]:PHASe:RESet</code>
DESCRIPTION	This command reset the phase offset display value of the RF output signal of the specified channel.
EQUIVALENT SCPI	<code>[:SOURce<ch>]:PHASe:REF</code>
EQUIVALENT MENU	FREQ > Reset phase delta display
EXAMPLE	<pre><i>:SOURce1:PHASe:RESet</i></pre>

3.4.3.6 Reset Phase ([:SOURce<ch>]:PHASe:REF)

SYNTAX	<code>[:SOURce<ch>]:PHASe:RESet</code>
DESCRIPTION	This command reset the phase offset display value of the RF output signal of the specified channel.
EQUIVALENT SCPI	<code>[:SOURce<ch>]:PHASe:RESet</code>

EQUIVALENT MENU	FREQ > Reset phase delta display
-----------------	---

EXAMPLE	<i>:SOURce1:PHASe:REF</i>
---------	---------------------------

3.4.3.7 Phase Memory ([[:SOURce<ch>]:PHASe:MEMory])

SYNTAX	[[:SOURce<ch>]:PHASe:MEMory ON OFF 1 0 [:SOURce<ch>]:PHASe:MEMory
--------	--

DESCRIPTION	This command sets/gets the phase memory switch status of the RF signal of the specified channel.
-------------	--

DATA TYPE	Boolean
-----------	---------

RANGE	ON OFF 1 0
-------	------------

RETURN	1 0
--------	-----

DEFAULT VALUE	0
---------------	---

EQUIVALENT MENU	FREQ > Phase Memory
-----------------	----------------------------

EXAMPLE	<i>:SOURce1:PHASe:MEMory 1</i> <i>:SOURce1:PHASe:MEMory?</i> Return: <i>1\n</i>
---------	--

3.4.3.8 Phase Memory Trigger ([[:SOURce<ch>]:PHASe:MEMory:TRIG])

SYNTAX	[[:SOURce<ch>]:PHASe:MEMory:TRIG
--------	----------------------------------

DESCRIPTION	This command triggers the RF phase memory function of the specified channel.
-------------	--

DATA TYPE	None
-----------	------

RANGE	ON OFF 1 0
-------	------------

RETURN	ON OFF 1 0
--------	------------

DEFAULT VALUE	None
---------------	------

EQUIVALENT MENU	FREQ > Phase Memory Trigger
-----------------	------------------------------------

EXAMPLE	<i>:SOURce1:PHASe:MEMory:TRIG</i>
---------	-----------------------------------

3.4.3.9 Phase Memory Parameter Query ([[:SOURce<ch>]:PHASe:MEMory:PARAM?])

SYNTAX	[[:SOURce<ch>]:PHASe:MEMory:PARAM?
--------	------------------------------------

DESCRIPTION	This command queries the stored parameters when the RF phase memory of the specified channel is triggered.
DATA TYPE	String
RANGE	None
	String Format: "Validity Status","Freq: <frequency_value>\nPhase: <phase_value>"\n
RETURN	Where: - Index: Integer (sweep point index) - Freq: Float (sweep point frequency, unit: Hz) - Level: Float (sweep point level, unit: dBm) - Time: Float (sweep point dwell time, unit: s)
DEFAULT VALUE	"Invalid","Freq:\s-1\nPhase:\s0"\n
EQUIVALENT MENU	FREQ > Phase Memory Trigger
EXAMPLE	<i>:SOURce1:PHASe:MEMory 1</i> <i>:SOURce1:PHASe:MEMory:TRIG</i> <i>:SOURce1:PHASe:MEMory:PARAM?</i> Return: <i>"Valid","Freq: 2e+10\nPhase: 0"\n</i>

3.4.4 Level

3.4.4.1 Level Display ([[:SOURce<ch>]:POWer:POWer])

SYNTAX	[[:SOURce<ch>]:POWer:POWer <power> [:SOURce<ch>]:POWer:POWer?
DESCRIPTION	This command sets/gets the level display value of the specified channel in the parameter bar at the top of the screen.
DATA TYPE	Float, unit: dBm, dBuV, uV, mV, V, nW, uW, mW or W, default is dBm
RETURN	Float, unit: dBm
DEFAULT VALUE	Minimum output level corresponding to the maximum output frequency
EQUIVALENT MENU	Level
EXAMPLE	<i>:SOURce1:POWer:POWer -2</i> <i>:SOURce1:POWer:POWer?</i>

```
:SOURce1:POWer:POWer -2
```

```
:SOURce1:POWer:POWer?
```

```
Return:
```

```
-2\n
```

3.4.4.2 Level ([:SOURce<ch>]:POWer)

SYNTAX	[:SOURce<ch>]:POWer <power> [:SOURce<ch>]:POWer?
DESCRIPTION	This command sets/gets the level of the RF output signal of the specified channel.
DATA TYPE	Float, unit: dBm, dBuV, uV, mV, V, nW, uW, mW or W, default is dBm
RANGE	Please refer to the datasheet
RETURN	Float, unit: dBm
DEFAULT VALUE	Minimum output level corresponding to the maximum output frequency
EQUIVALENT MENU	LEVEL > Level
EXAMPLE	<i>:SOURce1:POWer 2</i> <i>:SOURce1:POWer?</i> Return: <i>2\n</i>

3.4.4.3 Level ([:SOURce<ch>]:POWer[:LEVel][:IMMediate][:AMPLitude])

SYNTAX	[:SOURce<ch>]:POWer[:LEVel][:IMMediate][:AMPLitude] <power> [:SOURce<ch>]:POWer[:LEVel][:IMMediate][:AMPLitude]?
DESCRIPTION	This command sets/gets the level of the RF output signal of the specified channel.
DATA TYPE	Float, unit: dBm, dBuV, uV, mV, V, nW, uW, mW or W, default is dBm
RANGE	Please refer to the datasheet
RETURN	Float, unit: dBm
DEFAULT VALUE	Minimum output level corresponding to the maximum output frequency
EQUIVALENT MENU	LEVEL > Level
EXAMPLE	<i>:SOURce1:POWer:LEVel -5</i> <i>:SOURce1:POWer:LEVel?</i>

Return:

*-5ln***3.4.4.4 Level Offset ([:SOURce<ch>]:POWer:OFFSet)**

SYNTAX	[:SOURce<ch>]:POWer:OFFSet <power> [:SOURce<ch>]:POWer:OFFSet?
DESCRIPTION	This command sets/gets the level offset of the RF output signal of the specified channel.
DATA TYPE	Float, unit: dB
RANGE	-100 to 100
RETURN	Float, unit: dB
DEFAULT VALUE	0
EQUIVALENT MENU	LEVEL > Level Offset
EXAMPLE	<i>:SOURce1:POWer:OFFSet 2</i> <i>:SOURce1:POWer:OFFSet?</i> Return: <i>2ln</i>

3.4.4.5 ALC State ([:SOURce<ch>]:POWer:ALC)

SYNTAX	[:SOURce<ch>]:POWer:ALC ON OFF AUTO [:SOURce<ch>]:POWer:ALC?
DESCRIPTION	This command sets/gets the ALC state of the specified channel.
DATA TYPE	Enumeration
RANGE	ON OFF AUTO
RETURN	ON OFF AUTO
DEFAULT VALUE	AUTO
EQUIVALENT MENU	LEVEL > ALC State
EXAMPLE	<i>:SOURce1:POWer:ALC ON</i> <i>:SOURce1:POWer:ALC?</i> Return: <i>ONln</i>

3.4.4.6 Flatness List State ([:SOURce<ch>]:CORRection[:FLATness])

SYNTAX	<code>[:SOURce<ch>]:CORRection[:FLATness] ON OFF 1 0</code> <code>[:SOURce<ch>]:CORRection[:FLATness]?</code>
DESCRIPTION	This command sets/gets the state of flatness correction of the specified channel.
DATA TYPE	Boolean
RANGE	ON OFF 1 0
RETURN	1 0
DEFAULT VALUE	0
EQUIVALENT MENU	LEVEL > Flatness
EXAMPLE	<i><code>:SOURce1:CORRection:FLATness ON</code></i> <i><code>:SOURce1:CORRection?</code></i> Return: <i><code>1</code></i>

3.4.4.7 Flatness List Add Row ([:SOURce<ch>]:CORRection:FLATness:PAIR)

SYNTAX	<code>[:SOURce<ch>]:CORRection:FLATness:PAIR <freq>,<power></code>
DESCRIPTION	This command adds a line to the flatness list of the specified channel.
DATA TYPE	Freq: float, unit: Hz, kHz, MHz or GHz, default is Hz, Power: float, unit: dB
RANGE	Freq: Full frequency range, Power: -100 to 100
EQUIVALENT MENU	LEVEL > Flatness > Add
EXAMPLE	<i><code>:SOURce1:CORRection:FLATness:PAIR 3 MHz,-3</code></i>

3.4.4.8 Flatness List Delete Row ([:SOURce<ch>]:CORRection:FLATness:DELeTe)

SYNTAX	<code>[:SOURce<ch>]:CORRection:FLATness:DELeTe <row></code>
DESCRIPTION	This command removes a specified row from the flatness list of the specified channel.
DATA TYPE	Integer
RANGE	1 ~ total number of rows in the flatness list
EQUIVALENT MENU	LEVEL > Flatness > Delete

EXAMPLE *:SOURce1:CORRection:FLATness:DELeTe 1*

3.4.4.9 Flatness List Count ([[:SOURce<ch>]:CORRection:FLATness:COUNT?])

SYNTAX	[[:SOURce<ch>]:CORRection:FLATness:COUNT?
DESCRIPTION	This command queries the total number of rows of the flatness list of the specified channel.
RETURN	Integer
DEFAULT VALUE	0
EQUIVALENT MENU	LEVEL > Flatness
EXAMPLE	<i>:SOURce1:CORRection:FLATness:COUNT?</i> Return: <i>5\n</i>

3.4.4.10 Flatness List Store ([[:SOURce<ch>]:CORRection:STORE])

SYNTAX	[[:SOURce<ch>]:CORRection:STORE <"file_name">
DESCRIPTION	This command saves the flatness list of the specified channel into a file.
DATA TYPE	String
RANGE	None
EQUIVALENT MENU	LEVEL > Flatness > Save
EXAMPLE	<i>:SOURce1:CORRection:STORE "U-disk3/test.uflt"</i>

3.4.4.11 Flatness List Load ([[:SOURce<ch>]:CORRection:LOAD])

SYNTAX	[[:SOURce<ch>]:CORRection:LOAD <"file_name">
DESCRIPTION	This command loads the flatness list of the specified channel from a file.
DATA TYPE	String
RANGE	None
EQUIVALENT MENU	LEVEL > Flatness > Load
EXAMPLE	<i>:SOURce1:CORRection:LOAD "U-disk3/test.uflt"</i>

3.4.4.12 Flatness List Clear ([:SOURce<ch>]:CORRection:FLATness:PRESet)

SYNTAX	[:SOURce<ch>]:CORRection:FLATness:PRESet
DESCRIPTION	This command clears the flatness list of the specified channel.
EQUIVALENT MENU	LEVEL > Flatness > Clear
EXAMPLE	<i>:SOURce1:CORRection:FLATness:PRESet</i>

3.4.4.13 Flatness List Fill Type ([:SOURce<ch>]:CORRection:FLATness:FILL:TYPE)

SYNTAX	[:SOURce<ch>]:CORRection:FLATness:FILL:TYPE FLATness MANUal SWEEPlist [:SOURce<ch>]:CORRection:FLATness:FILL:TYPE?
DESCRIPTION	This command sets/gets the fill type of the flatness list of the specified channel.
DATA TYPE	Enumeration
RANGE	FLATness MANUal SWEEPlist
RETURN	Enumeration
DEFAULT VALUE	FLATness
EQUIVALENT MENU	LEVEL > Flatness > Setting > Fill Type
EXAMPLE	<i>:SOURce1:CORRection:FLATness:FILL:TYPE FLATness</i> <i>:SOURce1:CORRection:FLATness:FILL:TYPE?</i> Return: <i>FLATness\n</i>

3.4.4.14 Flatness List Start Freq ([:SOURce<ch>]:CORRection:FLATness:STARTfreq)

SYNTAX	[:SOURce<ch>]:CORRection:FLATness:STARTfreq <freq> [:SOURce<ch>]:CORRection:FLATness:STARTfreq?
DESCRIPTION	When the flatness list of the specified channel needs to be filled with a power sensor and the filling type is “Manual Step”, this command sets/queries the starting frequency of manual step filling.
DATA TYPE	Float, unit: Hz, kHz, MHz or GHz, default is Hz
RANGE	Full frequency range
RETURN	Float, unit: Hz
DEFAULT VALUE	Maximum frequency

EQUIVALENT MENU	LEVEL > Flatness > Setting > Fill Type (Manual Step) > Start Freq
EXAMPLE	<i>:SOURce1:CORRection:FLATness:STARTfreq 200 MHz</i> <i>:SOURce1:CORRection:FLATness:STARTfreq?</i> Return: <i>200000000\n</i>

3.4.4.15 Flatness List Stop Freq ([SOURce<ch>]:CORRection:FLATness:STOPfreq)

SYNTAX	[SOURce<ch>]:CORRection:FLATness:STOPfreq <freq> [SOURce<ch>]:CORRection:FLATness:STOPfreq?
DESCRIPTION	When the flatness list of the specified channel needs to be filled with a power sensor and the filling type is “Manual Step”, this command sets/queries the end frequency of manual step filling.
DATA TYPE	Float, unit: Hz, kHz, MHz or GHz, default is Hz
RANGE	Full frequency range
RETURN	Float, unit: Hz
DEFAULT VALUE	Maximum frequency
EQUIVALENT MENU	LEVEL > Flatness > Setting > Fill Type (Manual Step) > Stop Freq
EXAMPLE	<i>:SOURce1:CORRection:FLATness:STOPfreq 500 MHz</i> <i>:SOURce1:CORRection:FLATness:STOPfreq?</i> Return: <i>500000000\n</i>

3.4.4.16 Flatness List Fill Space ([SOURce<ch>]:CORRection:FLATness:SPACE)

SYNTAX	[SOURce<ch>]:CORRection:FLATness:SPACE LINear LOGarithmic [SOURce<ch>]:CORRection:FLATness:SPACE?
DESCRIPTION	When the flatness list needs to be filled with a power sensor and the filling type is “Manual Step”, this command sets/queries the frequency step method of manual step filling.
DATA TYPE	Enumeration
RANGE	LINear LOGarithmic
RETURN	Enumeration
DEFAULT VALUE	LINear
EQUIVALENT MENU	LEVEL > Flatness > Setting > Fill Type (Manual Step) > Fill Space

EXAMPLE *:SOURce1:CORRection:FLATness:SPACe LINear*
 :SOURce1:CORRection:FLATness:SPACe?
 Return:
 LINear\n

3.4.4.17 Flatness List Linear Step ([SOURce<ch>]:CORRection:FLATness:LINStep)

SYNTAX	[SOURce<ch>]:CORRection:FLATness:LINStep <freq> [SOURce<ch>]:CORRection:FLATness:LINStep?
DESCRIPTION	This command sets/queries the linear frequency step of manual step filling of the specified channel.
DATA TYPE	Float, unit: Hz, kHz, MHz or GHz, default is Hz
RETURN	Float, unit: Hz
DEFAULT VALUE	0
EQUIVALENT MENU	LEVEL > Flatness > Setting > Fill Type (Manual Step) > Step Linear
EXAMPLE	<i>:SOURce1:CORRection:FLATness:LINStep 200 MHz</i> <i>:SOURce1:CORRection:FLATness:LINStep?</i> Return: <i>200000000\n</i>

3.4.4.18 Flatness List Log Step ([SOURce<ch>]:CORRection:FLATness:LOGStep)

SYNTAX	[SOURce<ch>]:CORRection:FLATness:LOGStep <value> [SOURce<ch>]:CORRection:FLATness:LOGStep?
DESCRIPTION	This command sets/queries the logarithmic frequency step of manual step filling of the specified channel.
DATA TYPE	Float, unit: %
RETURN	Float, unit: %
DEFAULT VALUE	0
EQUIVALENT MENU	LEVEL > Flatness > Setting > Fill Type (Manual Step) > Step Log
EXAMPLE	<i>:SOURce1:CORRection:FLATness:LOGStep 20</i> <i>:SOURce1:CORRection:FLATness:LOGStep?</i> Return: <i>20\n</i>

3.4.4.19 Flatness List Points ([:SOURce<ch>]:CORRection:FLATness:POINT)

SYNTAX	[:SOURce<ch>]:CORRection:FLATness:POINT <points> [:SOURce<ch>]:CORRection:FLATness:POINT?
DESCRIPTION	This command sets/queries the sweep points of manual step filling Channel ch.
DATA TYPE	Integer
RANGE	2 to 500
RETURN	Integer
DEFAULT VALUE	2
EQUIVALENT MENU	LEVEL > Flatness > Setting > Fill Type (Manual Step) > Points
EXAMPLE	<i>:SOURce1:CORRection:FLATness:POINT 5</i> <i>:SOURce1:CORRection:FLATness:POINT?</i> Return: <i>5\n</i>

3.4.4.20 Fill Flatness with Sensor

([:SOURce<ch>]:CORRection:CSET:DATA[:SENSor][:POWer]:SONCe)

SYNTAX	[:SOURce<ch>]:CORRection:CSET:DATA[:SENSor][:POWer]:SONCe
DESCRIPTION	Amplitude correction values to populate flatness list with power sensor.
EQUIVALENT MENU	LEVEL > Flatness > Setting > Fill Flatness with Sensor
EXAMPLE	<i>:SOURce1:CORRection:CSET:DATA:SONCe</i>

3.4.5 Sweep

3.4.5.1 Sweep State ([:SOURce<ch>]:SWEep:STATe)

SYNTAX	[:SOURce<ch>]:SWEep:STATe OFFIFREQuency LEVellLEV_FREQ [:SOURce<ch>]:SWEep:STATe?
DESCRIPTION	This command sets/gets the sweep state of the specified channel.
DATA TYPE	Enumeration
RANGE	OFFIFREQuency LEVellLEV_FREQ
RETURN	Enumeration

DEFAULT VALUE	OFF
EQUIVALENT MENU	SWEEP > Sweep State
EXAMPLE	<pre><i>:SOURce1:SWEEp:STATe LEV_FREQ</i> <i>:SOURce1:SWEEp:STATe?</i></pre> Return: <pre><i>LEV_FREQ\n</i></pre>

3.4.5.2 Sweep Type ([[:SOURce<ch>]:SWEep:TYPE])

SYNTAX	<pre>[[:SOURce<ch>]:SWEep:TYPE LIST STEP [:SOURce<ch>]:SWEep:TYPE?</pre>
DESCRIPTION	This command sets the sweep type to step sweep or list sweep. This command queries whether the sweep type is step sweep or list sweep of the specified channel.
DATA TYPE	Enumeration
RANGE	LIST STEP
RETURN	Enumeration
DEFAULT VALUE	STEP
EQUIVALENT MENU	SWEEP > Step Sweep / List Sweep
EXAMPLE	<pre><i>:SOURce1:SWEEp:TYPE STEP</i> <i>:SOURce1:SWEEp:TYPE?</i></pre> Return: <pre><i>STEP\n</i></pre>

3.4.5.3 Start Frequency ([[:SOURce<ch>]:SWEep:STEP:START:FREQuency])

SYNTAX	<pre>[[:SOURce<ch>]:SWEep:STEP:START:FREQuency <freq> [:SOURce<ch>]:SWEep:STEP:START:FREQuency?</pre>
DESCRIPTION	This command sets/queries the starting frequency of step sweep of the specified channel.
DATA TYPE	Float, unit: Hz, kHz, MHz or GHz, default is Hz
RANGE	Full frequency range
RETURN	Float, unit: Hz
DEFAULT VALUE	Maximum frequency

EQUIVALENT MENU	SWEEP > Step Sweep > Start Freq
EXAMPLE	<pre> :SOURce1:SWEEP:STEP:START:FREQUENCY 1 GHz :SOURce1:SWEEP:STEP:START:FREQUENCY? Return: 10000000000\n </pre>

3.4.5.4 Stop Frequency ([[:SOURce<ch>]:SWEEP:STEP:STOP:FREQUENCY])

SYNTAX	<pre> [:SOURce<ch>]:SWEEP:STEP:STOP:FREQUENCY <freq> [:SOURce<ch>]:SWEEP:STEP:STOP:FREQUENCY? </pre>
DESCRIPTION	This command sets/queries the stop frequency of step sweep of the specified channel.
DATA TYPE	Float, unit: Hz, kHz, MHz or GHz, default is Hz
RANGE	Full frequency range
RETURN	Float, unit: Hz
DEFAULT VALUE	Maximum frequency
EQUIVALENT MENU	SWEEP > Step Sweep > Stop Freq
EXAMPLE	<pre> :SOURce1:SWEEP:STEP:STOP:FREQUENCY 1 GHz :SOURce1:SWEEP:STEP:STOP:FREQUENCY? Return: 10000000000\n </pre>

3.4.5.5 Start Level ([[:SOURce<ch>]:SWEEP:STEP:START:LEVEL])

SYNTAX	<pre> [:SOURce<ch>]:SWEEP:STEP:START:LEVEL <level> [:SOURce<ch>]:SWEEP:STEP:START:LEVEL? </pre>
DESCRIPTION	This command sets/queries the starting level of step sweep of the specified channel.
DATA TYPE	Float, unit: dBm, dBuV, uV, mV, V, nW, uW, mW or W, default is dBm
RANGE	Full level range
RETURN	Float, unit: dBm
DEFAULT VALUE	-130 dBm
EQUIVALENT MENU	SWEEP > Step Sweep > Start Level
EXAMPLE	<pre> :SOURce1:SWEEP:STEP:START:LEVEL 0 dBm </pre>

```
:SOURce1:SWEEp:STEP:START:LEVel?
```

```
Return:
```

```
0\n
```

3.4.5.6 Stop Level ([[:SOURce<ch>]:SWEep:STEP:STOP:LEVel])

SYNTAX	<pre>[[:SOURce<ch>]:SWEep:STEP:STOP:LEVel <level> [:SOURce<ch>]:SWEep:STEP:STOP:LEVel?</pre>
DESCRIPTION	This command sets/queries the stop level of step sweep of the specified channel.
DATA TYPE	Float, unit: dBm, dBuV, uV, mV, V, nW, uW, mW or W, default is dBm
RANGE	Full level range
RETURN	Float, unit: dBm
DEFAULT VALUE	-130 dBm
EQUIVALENT MENU	SWEEP > Step Sweep > Stop Level
EXAMPLE	<pre><i>:SOURce1:SWEEp:STEP:STOP:LEVel 0 dBm</i> <i>:SOURce1:SWEEp:STEP:STOP:LEVel?</i> Return: <i>0\n</i></pre>

3.4.5.7 Dwell Time ([[:SOURce<ch>]:SWEep:STEP:DWELI])

SYNTAX	<pre>[[:SOURce<ch>]:SWEep:STEP:DWELI <time> [:SOURce<ch>]:SWEep:STEP:DWELI?</pre>
DESCRIPTION	This command sets/queries the dwell time of step sweep of the specified channel.
DATA TYPE	Float, unit: ns, us, ms or s, default is s
RANGE	10 ms ~ 100 s
RETURN	Float, unit: s
DEFAULT VALUE	30 ms
EQUIVALENT MENU	SWEEP > Step Sweep > Dwell Time
EXAMPLE	<pre><i>:SOURce1:SWEEp:STEP:DWELI 20 ms</i> <i>:SOURce1:SWEEp:STEP:DWELI?</i> Return: <i>0.02\n</i></pre>

3.4.5.8 Sweep Points ([SOURce<ch>]:SWEep:STEP:POINTs)

SYNTAX	[SOURce<ch>]:SWEep:STEP:POINTs <points> [SOURce<ch>]:SWEep:STEP:POINTs?
DESCRIPTION	This command sets/queries the sweep points of step sweep of the specified channel.
DATA TYPE	Integer
RANGE	2 to 65535
RETURN	Integer
DEFAULT VALUE	11
EQUIVALENT MENU	SWEEP > Step Sweep > Sweep Points
EXAMPLE	<i>:SOURce1:SWEep:STEP:POINTs 2</i> <i>:SOURce1:SWEep:STEP:POINTs?</i> Return: <i>2\n</i>

3.4.5.9 Sweep Shape ([SOURce<ch>]:SWEep:STEP:SHAPE)

SYNTAX	[SOURce<ch>]:SWEep:STEP:SHAPE TRlangle SAWtooth [SOURce<ch>]:SWEep:STEP:SHAPE?
DESCRIPTION	This command sets/queries the sweep shape of step sweep of the specified channel.
DATA TYPE	Enumeration
RANGE	TRlangle SAWtooth
RETURN	Enumeration
DEFAULT VALUE	SAWtooth
EQUIVALENT MENU	SWEEP > Step Sweep > Sweep Shape
EXAMPLE	<i>:SOURce1:SWEep:STEP:SHAPE TRlangle</i> <i>:SOURce1:SWEep:STEP:SHAPE?</i> Return: <i>TRlangle\n</i>

3.4.5.10 Sweep Space ([SOURce<ch>]:SWEep:STEP:SPACE)

SYNTAX	[SOURce<ch>]:SWEep:STEP:SPACE LINear LOGarithmic [SOURce<ch>]:SWEep:STEP:SPACE?
--------	--

DESCRIPTION	This command sets/queries the frequency sweep space of step sweep of the specified channel.
DATA TYPE	Enumeration
RANGE	LINear LOGarithmic
RETURN	Enumeration
DEFAULT VALUE	LINear
EQUIVALENT MENU	SWEEP > Step Sweep > Sweep Space
EXAMPLE	<pre><i>:SOURce1:SWEEP:STEP:SPACE LOGarithmic</i> <i>:SOURce1:SWEEP:STEP:SPACE?</i></pre> Return: <pre><i>LOGarithmic\n</i></pre>

3.4.5.11 Linear Sweep Step ([:SOURce<ch>]:SWEEP[:FREQUENCY]:STEP[:LINear])

SYNTAX	[:SOURce<ch>]:SWEEP[:FREQUENCY]:STEP[:LINear] <freq> [:SOURce<ch>]:SWEEP[:FREQUENCY]:STEP[:LINear]?
DESCRIPTION	This command sets/queries the linear frequency step of the step sweep of the specified channel.
DATA TYPE	Float, unit: Hz, kHz, MHz or GHz, default is Hz
RETURN	Float, unit: Hz
DEFAULT VALUE	0
EQUIVALENT MENU	SWEEP > Step Sweep > Freq Step Linear
EXAMPLE	<pre><i>:SOURce1:SWEEP:STEP 200 MHz</i> <i>:SOURce1:SWEEP:STEP?</i></pre> Return: <pre><i>200000000\n</i></pre>

3.4.5.12 Logarithmic Sweep Step ([:SOURce<ch>]:SWEEP[:FREQUENCY]:STEP:LOGarithmic)

SYNTAX	[:SOURce<ch>]:SWEEP[:FREQUENCY]:STEP:LOGarithmic <value> [:SOURce<ch>]:SWEEP[:FREQUENCY]:STEP:LOGarithmic?
DESCRIPTION	This command sets/queries the logarithmic frequency step of the step sweep of the specified channel.
DATA TYPE	Float, unit: %
RETURN	Float, unit: %

DEFAULT VALUE	0
EQUIVALENT MENU	SWEEP > Step Sweep > Freq Step Log
EXAMPLE	<i>:SOURce1:SWEEp:STEP:LOGarithmic 20</i> <i>:SOURce1:SWEEp:STEP:LOGarithmic?</i> Return: <i>20ln</i>

3.4.5.13 Sweep List Add Row ([:SOURce<ch>]:SWEEp:LIST:ADDList)

SYNTAX	[:SOURce<ch>]:SWEEp:LIST:ADDList <freq>,<level>,<time>
DESCRIPTION	This command adds a line to the sweep list of the specified channel.
DATA TYPE	Freq: float, unit: Hz, kHz, MHz or GHz, default is Hz, Level: float, unit: dBm, dBuV, uV, mV, V, nW, uW, mW or W, default is dBm, Time: float, unit: ns, us, ms or s, default is s
RANGE	Freq: Full frequency range, Level: Full level range, Time: 10.0 ms ~ 100.0 s
EQUIVALENT MENU	SWEEP > List Sweep > Add
EXAMPLE	<i>:SOURce1:SWEEp:LIST:ADDList 1 GHz,0 dBm,1 s</i>

3.4.5.14 Sweep List Delete Row ([:SOURce<ch>]:SWEEp:LIST:DELeTe)

SYNTAX	[:SOURce<ch>]:SWEEp:LIST:DELeTe <row>
DESCRIPTION	This command removes a specified row from the sweep list of the specified channel.
DATA TYPE	Integer
RANGE	1 ~ total number of rows in the sweep list
EQUIVALENT MENU	SWEEP > List Sweep > Delete
EXAMPLE	<i>:SOURce1:SWEEp:LIST:DELeTe 1</i>

3.4.5.15 Sweep List Edit ([:SOURce<ch>]:SWEEp:LIST:CHANGe)

SYNTAX	[:SOURce<ch>]:SWEEp:LIST:CHANGe <row>,<freq>,<level>,<time>
DESCRIPTION	This command edits the specified row in the sweep list of the specified channel.

DATA TYPE	Row: Integer, Freq: float, unit: Hz, kHz, MHz or GHz, default is Hz, Level: float, unit: dBm, dBuV, uV, mV, V, nW, uW, mW or W, default is dBm, Time: float, unit: ns, us, ms or s, default is s
RANGE	Row: 1 ~ total number of rows in the sweep list, Freq: Full frequency range, Level: Full level range, Time: 10.0 ms ~ 100.0 s
EQUIVALENT MENU	SWEEP > List Sweep
EXAMPLE	<i><code>:SOURce1:SWEEp:LIST:CHANGe 1,1 GHz,1 dBm, 1 s</code></i>

3.4.5.16 Sweep List Count (`[[:SOURce<ch>]:SWEEp:LIST:CPOint?]`)

SYNTAX	<code>[[:SOURce<ch>]:SWEEp:LIST:CPOint?</code>
DESCRIPTION	This command queries the total number of rows of the sweep list of the specified channel.
RETURN	Integer
DEFAULT VALUE	1
EQUIVALENT MENU	SWEEP > List Sweep
EXAMPLE	<i><code>:SOURce1:SWEEp:LIST:CPOint?</code></i> Return: <i><code>5ln</code></i>

3.4.5.17 Sweep List Data (`[[:SOURce<ch>]:SWEEp:LIST:LIST?]`)

SYNTAX	<code>[[:SOURce<ch>]:SWEEp:LIST:LIST? <begin_row>,<end_row></code>
DESCRIPTION	This command queries the data from begin_row to end_row in the sweep list of the specified channel.
DATA TYPE	Integer, Integer
RANGE	1 ~ total number of rows in the sweep list, Start row ~ total number of rows in the sweep list
RETURN	String
EQUIVALENT MENU	SWEEP > List Sweep
EXAMPLE	<i><code>:SOURce1:SWEEp:LIST:LIST? 1,3</code></i>

Return:

*1000000000,0,0.03\s2000000000,-2.4,0.03\s3000000000,-
4.8,0.03\n*

3.4.5.18 Sweep List Clear ([:SOURce<ch>]:SWEep:LIST:INITialize:PRESet)

SYNTAX	[:SOURce<ch>]:SWEep:LIST:INITialize:PRESet
DESCRIPTION	This command clears the sweep list of the specified channel.
EQUIVALENT MENU	SWEEP > List Sweep > Clear
EXAMPLE	<i>[:SOURce1]:SWEep:LIST:INITialize:PRESet</i>

3.4.5.19 Sweep List Initialize From Step Sweep ([:SOURce<ch>]:SWEep:LIST:INITialize:FSTep)

SYNTAX	[:SOURce<ch>]:SWEep:LIST:INITialize:FSTep
DESCRIPTION	This command imports the sweep list from step sweep of the specified channel.
EQUIVALENT MENU	SWEEP > List Sweep > Import
EXAMPLE	<i>[:SOURce1]:SWEep:LIST:INITialize:FSTep</i>

3.4.5.20 Sweep List Load ([:SOURce<ch>]:SWEep:LOAD)

SYNTAX	[:SOURce<ch>]:SWEep:LOAD <"file_name">
DESCRIPTION	This command loads the sweep list of the specified channel from the file.
DATA TYPE	String
RANGE	None
EQUIVALENT MENU	SWEEP > List Sweep > Load
EXAMPLE	<i>[:SOURce1]:SWEep:LOAD "U-disk3/test.lsw"</i>

3.4.5.21 Sweep List Store ([:SOURce<ch>]:SWEep:STORe)

SYNTAX	[:SOURce<ch>]:SWEep:STORe <"file_name">
DESCRIPTION	This command saves the sweep list of the specified channel into a file.
DATA TYPE	String

RANGE	None
EQUIVALENT MENU	SWEEP > List Sweep > Save
EXAMPLE	<i>:SOURce1:SWEEp:STORe "U-disk3/test.lsw"</i>

3.4.5.22 Sweep Direction ([[:SOURce<ch>]:SWEEp:DIRect)

SYNTAX	[[:SOURce<ch>]:SWEEp:DIRect FWD REV [:SOURce<ch>]:SWEEp:DIRect?
DESCRIPTION	This command sets/queries the sweep direction of the specified channel.
DATA TYPE	Enumeration
RANGE	FWD REV
RETURN	Enumeration
DEFAULT VALUE	FWD
EQUIVALENT MENU	SWEEP > Direction
EXAMPLE	<i>:SOURce1:SWEEp:DIRect REV</i> <i>:SOURce1:SWEEp:DIRect?</i> Return: <i>REVn</i>

3.4.5.23 Sweep Mode ([[:SOURce<ch>]:SWEEp:MODE)

SYNTAX	[[:SOURce<ch>]:SWEEp:MODE CONTInue SINGle [:SOURce<ch>]:SWEEp:MODE?
DESCRIPTION	This command sets the sweep mode of the specified channel to continuous or single. This command queries the sweep mode of the specified channel.
DATA TYPE	Enumeration
RANGE	CONTInue SINGle
RETURN	Enumeration
DEFAULT VALUE	CONTInue
EQUIVALENT MENU	SWEEP > Sweep Mode
EXAMPLE	<i>:SOURce1:SWEEp:MODE SINGle</i> <i>:SOURce1:SWEEp:MODE?</i>

Return:
SINGleIn

3.4.5.24 Execute Single Sweep ([:SOURce<ch>]:SWEep:EXECute)

SYNTAX	[:SOURce<ch>]:SWEep:EXECute
DESCRIPTION	When the sweep mode of the specified channel is single, this command can perform a single sweep.
EQUIVALENT MENU	SWEEP > Execute single sweep
EXAMPLE	<i>:SOURce1:SWEep:EXECute</i>

3.4.5.25 Trigger Mode ([:SOURce<ch>]:SWEep:SWEep:TRIGger:TYPE)

SYNTAX	[:SOURce<ch>]:SWEep:SWEep:TRIGger:TYPE AUTO KEY BUS EXT [:SOURce<ch>]:SWEep:SWEep:TRIGger:TYPE?
DESCRIPTION	This command sets/queries the sweep trigger mode of the specified channel.
DATA TYPE	Enumeration
RANGE	AUTO KEY BUS EXT
RETURN	Enumeration
DEFAULT VALUE	AUTO
EQUIVALENT MENU	SWEEP > Trigger Mode
EXAMPLE	<i>:SOURce1:SWEep:SWEep:TRIGger:TYPE KEY</i> <i>:SOURce1:SWEep:SWEep:TRIGger:TYPE?</i> Return: <i>KEYIn</i>

3.4.5.26 Point Trigger ([:SOURce<ch>]:SWEep:POINT:TRIGger:TYPE)

SYNTAX	[:SOURce<ch>]:SWEep:POINT:TRIGger:TYPE AUTO KEY BUS EXT [:SOURce<ch>]:SWEep:POINT:TRIGger:TYPE?
DESCRIPTION	This command sets/queries the point sweep trigger mode of the specified channel.
DATA TYPE	Enumeration
RANGE	AUTO KEY BUS EXT

RETURN	Enumeration
DEFAULT VALUE	AUTO
EQUIVALENT MENU	SWEEP > Point Trigger
EXAMPLE	<pre> :<i>SOURce1:SWEEp:POINt:TRIGger:TYPE KEY</i> :<i>SOURce1:SWEEp:POINt:TRIGger:TYPE?</i> Return: <i>KEYIn</i> </pre>

3.4.5.27 Trigger Slope ([*:SOURce<ch>*]:*INPut:TRIGger:SLOPe*)

SYNTAX	<pre> [<i>:SOURce<ch></i>]:<i>INPut:TRIGger:SLOPe POSitive NEGative</i> [<i>:SOURce<ch></i>]:<i>INPut:TRIGger:SLOPe?</i> </pre>
DESCRIPTION	This command sets/queries the trigger edge of the external trigger signal for the sweep function of the specified channel.
DATA TYPE	Enumeration
RANGE	POSitive NEGative
RETURN	Enumeration
DEFAULT VALUE	POSitive
EQUIVALENT MENU	SWEEP > Trigger Slope
EXAMPLE	<pre> :<i>SOURce1:INPut:TRIGger:SLOPe NEGative</i> :<i>SOURce1:INPut:TRIGger:SLOPe?</i> Return: <i>NEGativeIn</i> </pre>

3.4.5.28 Get Current Sweep Point ([*:SOURce<ch>*]:*SWEEp:CURRent:DATA?*)

SYNTAX	<i>:SOURce<ch></i> : <i>SWEEp:CURRent:DATA?</i>
DESCRIPTION	This command queries the current sweep point of the specified channel.
RETURN	String The string format: index,{freq,level,time} Index: interger, Freq: float, unit: Hz, Level: float, unit: dBm, Time: float, unit: s.

DEFAULT VALUE	None
EQUIVALENT MENU	Display frequency and display level at the top of the screen
EXAMPLE	<i>:SOURce1:SWEEp:CURRent:DATA?</i> Return: <i>1,{1000000000,0,0.03}\n</i>

3.4.5.29 Get the Frequency of the Current Sweep Point ([:SOURce<ch>]:SWEEp:CURRent:FREQuency?)

SYNTAX	<code>[[:SOURce<ch>]:SWEEp:CURRent:FREQuency?</code>
DESCRIPTION	This command queries the frequency of the current sweep point of the specified channel.
RETURN	Float, unit: Hz
DEFAULT VALUE	None
EQUIVALENT MENU	Display frequency at the top of the screen
EXAMPLE	<i>:SOURce1:SWEEp:CURRent:FREQuency?</i> Return: <i>1000000000.000000\n</i>

3.4.5.30 Get the Level of the Current Sweep Point ([:SOURce<ch>]:SWEEp:CURRent:LEVel?)

SYNTAX	<code>[[:SOURce<ch>]:SWEEp:CURRent:LEVel?</code>
DESCRIPTION	This command queries the level of the current sweep point of the specified channel.
RETURN	Float, unit: dBm
DEFAULT VALUE	None
EQUIVALENT MENU	Display level at the top of the screen
EXAMPLE	<i>:SOURce1:SWEEp:CURRent:LEVel?</i> Return: <i>0.000000\n</i>

3.4.6 Sensor

3.4.6.1 Level Control ([:SOURce]:POWer:SPC:STATe)

SYNTAX	[:SOURce]:POWer:SPC:STATe ON OFF 1 0 [:SOURce]:POWer:SPC:STATe?
DESCRIPTION	This command sets/queries the level control state of the power sensor.
DATA TYPE	Boolean
RANGE	ON OFF 1 0
RETURN	1 0
DEFAULT VALUE	0
EQUIVALENT SCPI	:SENSe[:POWer]:LEV:CTL:STATe ON OFF 1 0 :SENSe[:POWer]:LEV:CTL:STATe?
EQUIVALENT MENU	 >  >  > Level Control
EXAMPLE	<i>:POWer:SPC:STATe ON</i> <i>:POWer:SPC:STATe?</i> Return: <i>1</i>

3.4.6.2 Channel Level Control ([:SOURce<ch>]:POWer:SPC:STATe)

SYNTAX	[:SOURce<ch>]:POWer:SPC:STATe ON OFF 1 0 [:SOURce<ch>]:POWer:SPC:STATe?
DESCRIPTION	This command sets/queries the level control state of the power sensor of the specified channel.
DATA TYPE	Boolean
RANGE	ON OFF 1 0
RETURN	1 0
DEFAULT VALUE	0
EQUIVALENT SCPI	:SENSe[:POWer]:LEV:CTL:STATe ON OFF 1 0 :SENSe[:POWer]:LEV:CTL:STATe?
EQUIVALENT MENU	 >  >  > Level Control
EXAMPLE	<i>:SOURce1:POWer:SPC:STATe ON</i>

```
:SOURce1:POWer:SPC:STATe?
```

Return:

```
1\n
```

3.4.6.3 Target Level ([:SOURce]:POWer:SPC:TARGet)

SYNTAX	<code>[:SOURce]:POWer:SPC:TARGet <power></code> <code>[:SOURce]:POWer:SPC:TARGet?</code>
DESCRIPTION	This command sets/queries the target level of the power sensor level control.
DATA TYPE	Float, unit: dBm, dBuV, uV, mV, V, nW, uW, mW or W, default is dBm
RANGE	-120 dBm ~ 20 dBm
RETURN	Float, unit: dBm
DEFAULT VALUE	0
EQUIVALENT SCPI	<code>:SENSe[:POWer]:SPC:TARGet <power></code> <code>:SENSe[:POWer]:SPC:TARGet?</code>
EQUIVALENT MENU	 >  >  > Level Control > Target Level
EXAMPLE	<pre><i>:POWer:SPC:TARGet 0</i></pre> <pre><i>:POWer:SPC:TARGet?</i></pre> Return: <pre><i>0\n</i></pre>

3.4.6.4 Limit Level ([:SOURce]:POWer:LIMit)

SYNTAX	<code>[:SOURce]:POWer:LIMit <power></code> <code>[:SOURce]:POWer:LIMit?</code>
DESCRIPTION	This command sets/queries the Limit level of the power sensor level control.
DATA TYPE	Float, unit: dBm, dBuV, uV, mV, V, nW, uW, mW or W, default is dBm
RANGE	-120 dBm ~ 20 dBm
RETURN	Float, unit: dBm
DEFAULT VALUE	0
EQUIVALENT SCPI	<code>:SENSe[:POWer]:LIMit <power></code> <code>:SENSe[:POWer]:LIMit?</code>

EQUIVALENT MENU

HOME >  >  > Level Control > Limit Level

EXAMPLE

POWer:LiMit 1

POWer:LiMit?

Return:

1ln

3.4.6.5 Catch Range ([:SOURce]:POWer:SPC:CRANge)

SYNTAX

[SOURce]:POWer:SPC:CRANge <power>
[SOURce]:POWer:SPC:CRANge?

DESCRIPTION

This command sets/queries the catch range of the power sensor level control.

DATA TYPE

Float, unit: dB

RANGE

0 ~ 50

RETURN

Float, unit: dB

DEFAULT VALUE

0

EQUIVALENT SCPI

:SENSe[:POWer]:SPC:CRANge <power>
:SENSe[:POWer]:SPC:CRANge?

EQUIVALENT MENU

HOME >  >  > Level Control > Catch Range

EXAMPLE

:POWer:SPC:CRANge 5

:POWer:SPC:CRANge?

Return:

5ln

3.4.7 Analog Modulation

3.4.7.1 Analog Modulation State ([:SOURce<ch>]:MODulation)

SYNTAX

[[:SOURce<ch>]:MODulation ON|OFF|1|0
[:SOURce<ch>]:MODulation?

DESCRIPTION

This command sets/gets the switch status of analog modulation of the specified channel.

DATA TYPE

Boolean

RANGE

ON|OFF|1|0

RETURN	1 0
DEFAULT VALUE	0
EQUIVALENT SCPI	:OUTPut:MODulation[:STATe] ON OFF 1 0 :OUTPut:MODulation[:STATe]?
EQUIVALENT MENU	ANALOG MOD > On
EXAMPLE	<i>:SOURce1:MODulation ON</i> <i>:SOURce1:MODulation?</i> Return: <i>1\n</i>

3.4.7.2 FM

3.4.7.2.1 FM State ([:SOURce<ch>]:FM:STATe)

SYNTAX	[[:SOURce<ch>]:FM:STATe ON OFF 1 0 [:SOURce<ch>]:FM:STATe?
DESCRIPTION	This command sets/gets the switch status of FM of the specified channel.
DATA TYPE	Boolean
RANGE	ON OFF 1 0
RETURN	1 0
DEFAULT VALUE	0
EQUIVALENT MENU	Analog Mod > FM > FM State
EXAMPLE	<i>:FM:STATe ON</i> <i>:FM:STATe?</i> Return: <i>1\n</i>

3.4.7.2.2 FM Source ([:SOURce<ch>]:FM:SOURce)

SYNTAX	[[:SOURce<ch>]:FM:SOURce INT1 INT2 INT1,INT2 EXTErnal INT1,EXTIDUAL [:SOURce<ch>]:FM:SOURce?
DESCRIPTION	This command sets/gets the modulation source of FM of the specified channel.
DATA TYPE	Enumeration

RANGE	INT1 INT2 INT1,INT2 EXTErnal INT1,EXTIDUAL
RETURN	Enumeration
DEFAULT VALUE	INT1
EQUIVALENT MENU	Analog Mod > FM > FM Source
EXAMPLE	<i>:FM:SOURce EXT</i> <i>:FM:SOURce?</i> Return: <i>EXTErnal\n</i>

3.4.7.2.3 FM Shape1 ([:SOURce<ch>]:FM1:WAVEform)

SYNTAX	[[:SOURce<ch>]:FM1:WAVEform SINE SQUare SAWTooth TRLangle [:SOURce<ch>]:FM1:WAVEform?
DESCRIPTION	This command sets/gets the FM waveform of INT1 of the specified channel.
DATA TYPE	Enumeration
RANGE	SINE SQUare SAWTooth TRLangle
RETURN	Enumeration
DEFAULT VALUE	SINE
EQUIVALENT MENU	Analog Mod > FM > FM Shape 1
EXAMPLE	<i>:FM1:WAVEform SQUare</i> <i>:FM1:WAVEform?</i> Return: <i>SQUare\n</i>

3.4.7.2.4 FM Deviation1 ([:SOURce<ch>]:FM1:DEViation)

SYNTAX	[[:SOURce<ch>]:FM1:DEViation <value> [:SOURce<ch>]:FM1:DEViation?
DESCRIPTION	This command sets/gets the FM deviation value of INT1 of the specified channel.
DATA TYPE	Float, unit: Hz, kHz, MHz or GHz, default is Hz
RANGE	1 Hz ~ N*1 MHz, N is the frequency segment coefficient, please refer to the data sheet
RETURN	Float, unit: Hz

DEFAULT VALUE	100kHz
EQUIVALENT MENU	Analog Mod > FM > FM Deviation 1
EXAMPLE	<i>:FM1:DEVIation 500 kHz</i> <i>:FM1:DEVIation?</i> Return: <i>500000\n</i>

3.4.7.2.5 FM Rate 1 ([[:SOURce<ch>]:FM1:FREQuency)

SYNTAX	<i>[[:SOURce<ch>]:FM1:FREQuency <value></i> <i>[[:SOURce<ch>]:FM1:FREQuency?</i>
DESCRIPTION	This command sets/gets the FM modulation rate of INT1 of the specified channel.
DATA TYPE	Float, unit: Hz, kHz, MHz or GHz, default is Hz
RANGE	1 Hz ~ N*1 MHz, N is the frequency segment coefficient, please refer to the data sheet
RETURN	Float, unit: Hz
DEFAULT VALUE	10kHz
EQUIVALENT MENU	Analog Mod > FM > FM Rate 1
EXAMPLE	<i>:FM1:FREQuency 40 kHz</i> <i>:FM1:FREQuency?</i> Return: <i>40000\n</i>

3.4.7.2.6 FM Phase1 ([[:SOURce<ch>]:FM1:PHASe)

SYNTAX	<i>[[:SOURce<ch>]:FM1:PHASe <value></i> <i>[[:SOURce<ch>]:FM1:PHASe?</i>
DESCRIPTION	When the frequency modulation source of the specified channel is internal source 1 + internal source 2 (Int1 + Int2) or Dual waveform, this command sets/queries the initial phase of INT1.
DATA TYPE	Float, unit: degree (°)
RANGE	-360 ~ +360
RETURN	Float, unit: degree (°)
DEFAULT VALUE	0

EQUIVALENT MENU	Analog Mod > FM > FM Phase 1
EXAMPLE	<i>:FM1:PHASe -30</i> <i>:FM1:PHASe?</i> Return: <i>-30\n</i>

3.4.7.2.7 FM Shape2 ([:SOURce<ch>]:FM2:WAVeform)

SYNTAX	[:SOURce<ch>]:FM2:WAVeform SINE SQUare SAWTooth TRlangle [:SOURce<ch>]:FM2:WAVeform?
DESCRIPTION	This command sets/gets the FM waveform of INT2 of the specified channel.
DATA TYPE	Enumeration
RANGE	SINE SQUare SAWTooth TRlangle
RETURN	Enumeration
DEFAULT VALUE	SINE
EQUIVALENT MENU	Analog Mod > FM > FM Shape 2
EXAMPLE	<i>:FM2:WAVeform TRlangle</i> <i>:FM2:WAVeform?</i> Return: <i>TRlangle\n</i>

3.4.7.2.8 FM Deviation2 ([:SOURce<ch>]:FM2:DEViation)

SYNTAX	[:SOURce<ch>]:FM2:DEViation <value> [:SOURce<ch>]:FM2:DEViation?
DESCRIPTION	This command sets/gets the FM deviation value of INT2 of the specified channel.
DATA TYPE	Float, unit: Hz, kHz, MHz or GHz, default is Hz
RANGE	1 Hz ~ N*1 MHz, N is the frequency segment coefficient, please refer to the data sheet
RETURN	Float, unit: Hz
DEFAULT VALUE	100kHz
EQUIVALENT MENU	Analog Mod > FM > FM Deviation 2
EXAMPLE	<i>:FM2:DEViation 500 kHz</i>

```
:FM2:DEVIation?
```

Return:

```
500000\n
```

3.4.7.2.9 FM Rate 2 ([[:SOURce<ch>]:FM2:FREQuency])

SYNTAX	[[:SOURce<ch>]:FM2:FREQuency <value> [:SOURce<ch>]:FM2:FREQuency?
DESCRIPTION	This command sets/gets the FM modulation rate of INT2 of the specified channel.
DATA TYPE	Float, unit: Hz, kHz, MHz or GHz, default is Hz
RANGE	1 Hz ~ N*1 MHz, N is the frequency segment coefficient, please refer to the data sheet
RETURN	Float, unit: Hz
DEFAULT VALUE	10kHz
EQUIVALENT MENU	Analog Mod > FM > FM Rate 2
EXAMPLE	<i>:FM2:FREQuency 40 kHz</i> <i>:FM2:FREQuency?</i> Return: <i>40000\n</i>

3.4.7.2.10 FM Phase2 ([[:SOURce<ch>]:FM2:PHASe])

SYNTAX	[[:SOURce<ch>]:FM2:PHASe <value> [:SOURce<ch>]:FM2:PHASe?
DESCRIPTION	When the frequency modulation source of the specified channel is internal source 1 + internal source 2 (Int1 + Int2) or Dual waveform, this command sets/queries the initial phase of INT2.
DATA TYPE	Float, unit: degree (°)
RANGE	-360 ~ +360
RETURN	Float, unit: degree (°)
DEFAULT VALUE	0
EQUIVALENT MENU	Analog Mod > FM > FM Phase 2
EXAMPLE	<i>:FM2:PHASe -30 deg</i> <i>:FM2:PHASe?</i>

Return:

*-30\n***3.4.7.2.11 Int1 Proportion ([[:SOURce<ch>]:FM1:PROPortion)**

SYNTAX	[[:SOURce<ch>]:FM1:PROPortion <value> [:SOURce<ch>]:FM1:PROPortion?
DESCRIPTION	When the FM Source of the specified channel is Dual, this command sets/queries the amplitude proportion of Int1.
DATA TYPE	Float
RANGE	0 ~ 1
RETURN	Float
DEFAULT VALUE	0.5
EQUIVALENT MENU	Analog Mod > FM > Int1 Proportion
EXAMPLE	<i>:FM1:PROPortion 0.6</i> <i>:FM1:PROPortion?</i> Return: <i>0.6\n</i>

3.4.7.2.12 FM Sensitivity1 ([[:SOURce<ch>]:FM1:SENSitivity?])

SYNTAX	[[:SOURce<ch>]:FM1:SENSitivity?
DESCRIPTION	When FM source of the specified channel includes an external source, this command queries the sensitivity of the external source input.
RETURN	Float, unit: Hz/V
DEFAULT VALUE	None
EQUIVALENT MENU	Analog Mod > FM > FM Sensitivity1
EXAMPLE	<i>:FM1:SENSitivity?</i> Return: <i>125000\n</i>

3.4.7.3 PM**3.4.7.3.1 PM State ([[:SOURce<ch>]:PM:STATe])**

SYNTAX	[[:SOURce<ch>]:PM:STATe ON OFF 1 0 [:SOURce<ch>]:PM:STATe?
--------	---

DESCRIPTION	This command sets/gets the switch status of PM of the specified channel.
DATA TYPE	Boolean
RANGE	ON OFF 1 0
RETURN	1 0
DEFAULT VALUE	0
EQUIVALENT MENU	Analog Mod > PM > PM State
EXAMPLE	<i>:PM:STATe ON</i> <i>:PM:STATe?</i> Return: <i>1ln</i>

3.4.7.3.2 PM Shape ([:SOURce<ch>]:PM:WAVEform)

SYNTAX	<i>[:SOURce<ch>]:PM:WAVEform SINE SQUare SAWTooth TRiangle</i> <i>[:SOURce<ch>]:PM:WAVEform?</i>
DESCRIPTION	This command sets/gets the PM waveform of the specified channel.
DATA TYPE	Enumeration
RANGE	SINE SQUare SAWTooth TRiangle
RETURN	Enumeration
DEFAULT VALUE	SINE
EQUIVALENT MENU	Analog Mod > PM > PM Shape
EXAMPLE	<i>:PM:WAVEform SQUare</i> <i>:PM:WAVEform?</i> Return: <i>SQUareln</i>

3.4.7.3.3 PM Source ([:SOURce<ch>]:PM:SOURce)

SYNTAX	<i>[:SOURce<ch>]:PM:SOURce</i> <i>INT1 INT2 INT1,INT2 EXTErnal INT1,EXTIDUAL</i> <i>[:SOURce<ch>]:PM:SOURce?</i>
DESCRIPTION	This command sets/gets the modulation source of PM of the specified channel.
DATA TYPE	Enumeration

RANGE	INTernal EXTernal INT,EXT
RETURN	Enumeration
DEFAULT VALUE	INTernal
EQUIVALENT MENU	Analog Mod > PM > PM Source
EXAMPLE	<i>:PM:SOURce EXTernal</i> <i>:PM:SOURce?</i> Return: <i>EXTernal\n</i>

3.4.7.3.4 PM Deviation ([[:SOURce<ch>]:PM:DEViation)

SYNTAX	<i>[[:SOURce<ch>]:PM:DEViation <value></i> <i>[[:SOURce<ch>]:PM:DEViation?</i>
DESCRIPTION	This command sets/gets the PM deviation value of INT1 of the specified channel.
DATA TYPE	Float, unit: rad
RANGE	0.01 rad ~ N*5 rad, N is the frequency segment coefficient, please refer to the data sheet
RETURN	Float, unit: rad
DEFAULT VALUE	1
EQUIVALENT MENU	Analog Mod > PM > PM Deviation
EXAMPLE	<i>:PM:DEViation 2</i> <i>:PM:DEViation?</i> Return: <i>2\n</i>

3.4.7.3.5 PM Rate ([[:SOURce<ch>]:PM:FREQuency)

SYNTAX	<i>[[:SOURce<ch>]:PM:FREQuency <value></i> <i>[[:SOURce<ch>]:PM:FREQuency?</i>
DESCRIPTION	This command sets/gets the PM modulation rate of the specified channel.
DATA TYPE	Float, unit: Hz, kHz, MHz or GHz, default is Hz
RANGE	Modulation wave is Sine: 0.01 Hz ~ 100 kHz, Modulation wave is Square: 0.01 Hz ~ 20 kHz.

RETURN	Float, unit: Hz
DEFAULT VALUE	10 kHz
EQUIVALENT MENU	Analog Mod > PM > PM Rate
EXAMPLE	<i>:PM:FREQuency 1 kHz</i> <i>:PM:FREQuency?</i> Return: <i>1000\n</i>

3.4.7.3.6 PM Sensitivity ([:SOURce<ch>]:PM:SENSitivity?)

SYNTAX	<code>[[:SOURce<ch>]:PM:SENSitivity?</code>
DESCRIPTION	When PM source of the specified channel includes an external source, this command queries the sensitivity of external source input.
RETURN	Float, unit: rad/V
DEFAULT VALUE	None
EQUIVALENT MENU	Analog Mod > PM > PM Sensitivity
EXAMPLE	<i>:PM:SENSitivity?</i> Return: <i>0.25\n</i>

3.4.8 Pulse Modulation

3.4.8.1 Pulse State ([:SOURce<ch>]:PULM:STATe)

SYNTAX	<code>[[:SOURce<ch>]:PULM:STATe ON OFF 1 0</code> <code>[[:SOURce<ch>]:PULM:STATe?</code>
DESCRIPTION	This command sets/gets the switch status of pulse modulation of the specified channel.
DATA TYPE	Boolean
RANGE	ON OFF 1 0
RETURN	1 0
DEFAULT VALUE	0
EQUIVALENT MENU	MOD > PULSE > Pulse State
EXAMPLE	<i>:SOURce1:PULM:STATe ON</i> <i>:SOURce1:PULM:STATe?</i>

Return:

*1\n***3.4.8.2 Pulse Source ([:SOURce<ch>]:PULM:SOURce)**

SYNTAX	<code>[[:SOURce<ch>]:PULM:SOURce INTernal EXTernal [:SOURce<ch>]:PULM:SOURce?</code>
DESCRIPTION	This command sets/queries the modulation source of pulse modulation of the specified channel.
DATA TYPE	Enumeration
RANGE	INTernal EXTernal
RETURN	Enumeration
DEFAULT VALUE	INTernal
EQUIVALENT SCPI	<code>[[:SOURce<ch>]:PULM:SOURce:INT INTernal EXTernal [:SOURce<ch>]:PULM:SOURce:INT?</code>
EQUIVALENT MENU	Analog Mod > PULSE > Pulse Source
EXAMPLE	<i><code>:SOURce1:PULM:SOURce INTernal</code> <code>:SOURce1:PULM:SOURce?</code> Return: <i><code>INTernal\n</code></i></i>

3.4.8.3 Pulse Source ([:SOURce <ch>]:PULM:SOURce:INT)

SYNTAX	<code>[[:SOURce <ch>]:PULM:SOURce:INT INTernal EXTernal [:SOURce <ch>]:PULM:SOURce:INT?</code>
DESCRIPTION	This command sets/queries the modulation source of pulse modulation of the specified channel.
DATA TYPE	Enumeration
RANGE	INTernal EXTernal
RETURN	Enumeration
DEFAULT VALUE	INTernal
EQUIVALENT SCPI	<code>[[:SOURce<ch>]:PULM:SOURce INTernal EXTernal [:SOURce<ch>]:PULM:SOURce?</code>
EQUIVALENT MENU	Analog Mod > PULSE > Pulse Source
EXAMPLE	<i><code>:SOURce1:PULM:SOURce:INT EXTernal</code></i>

```
:SOURce1:PULM:SOURce:INT?
```

```
Return:
```

```
EXternal\n
```

3.4.8.3.1 Pulse Out ([[:SOURce<ch>]:PULM:OUT:STATE])

SYNTAX	[[:SOURce<ch>]:PULM:OUT:STATE ON OFF 1 0 [:SOURce<ch>]:PULM:OUT:STATE?
DESCRIPTION	This command sets/queries the pulse output status of pulse modulation of the specified channel.
DATA TYPE	Boolean
RANGE	ON OFF 1 0
RETURN	1 0
DEFAULT VALUE	0
EQUIVALENT MENU	Analog Mod > PULSE > Pulse Out
EXAMPLE	<i>:SOURce1:PULM:OUT:STATE ON</i> <i>:SOURce1:PULM:OUT:STATE?</i> Return: <i>1\n</i>

3.4.8.3.2 Pulse Out Polarity ([[:SOURce<ch>]:PULM:POLarity])

SYNTAX	[[:SOURce<ch>]:PULM:POLarity NORMal INVerted [:SOURce<ch>]:PULM:POLarity?
DESCRIPTION	This command sets/queries the pulse output polarity of the specified channel.
DATA TYPE	Enumeration
RANGE	NORMal INVerted
RETURN	Enumeration
DEFAULT VALUE	NORMal
EQUIVALENT MENU	Analog Mod > PULSE > Pulse Out Polarity
EXAMPLE	<i>:SOURce1:PULM:POL INV</i> <i>:SOURce1:PULM:POLarity?</i> Return: <i>INVerted\n</i>

3.4.8.3.3 Pulse Mode ([:SOURce<ch>]:PULM:MODE)

SYNTAX	[:SOURce<ch>]:PULM:MODE SINGLE DOUBLE PTRain [:SOURce<ch>]:PULM:MODE?
DESCRIPTION	This command sets the pulse mode of the specified channel to Single pulse, Double pulse or pulse Train. This command queries the pulse mode of the specified channel.
DATA TYPE	Enumeration
RANGE	SINGLE DOUBLE PTRain
RETURN	Enumeration
DEFAULT VALUE	SINGLE
EQUIVALENT MENU	Analog Mod > PULSE > Pulse Mode
EXAMPLE	<i>[:SOURce1:PULM:MODE DOUB</i> <i>[:SOURce1:PULM:MODE?</i> Return: <i>DOUBLE</i>

3.4.8.3.4 Pulse Period ([:SOURce<ch>]:PULM:PERiod)

SYNTAX	[:SOURce<ch>]:PULM:PERiod <value> [:SOURce<ch>]:PULM:PERiod?
DESCRIPTION	When the pulse mode of the specified channel is Single or Double, this command sets/queries the pulse period.
DATA TYPE	Float, unit: ns, us, ms or s, default is s
RANGE	40 ns ~ 300 s
RETURN	Float, unit: s
DEFAULT VALUE	10 ms
EQUIVALENT SCPI	[:SOURce<ch>]:PULM:INT[1]:PERiod <value> [:SOURce<ch>]:PULM:INT[1]:PERiod?
EQUIVALENT MENU	Analog Mod > PULSE > Pulse Period
EXAMPLE	<i>[:SOURce1:PULM:PER 220 us</i> <i>[:SOURce1:PULM:PER?</i> Return: <i>0.00022</i>

3.4.8.3.5 Pulse Period ([:SOURce<ch>]:PULM:INT[1]:PERiod)

SYNTAX	[:SOURce<ch>]:PULM:INT[1]:PERiod <value> [:SOURce<ch>]:PULM:INT[1]:PERiod?
DESCRIPTION	When the pulse mode of the specified channel is Single or Double, this command sets/queries the pulse period.
DATA TYPE	Float, unit: ns, us, ms or s, default is s
RANGE	40 ns ~ 300 s
RETURN	Float, unit: s
DEFAULT VALUE	10 ms
EQUIVALENT SCPI	[:SOURce<ch>]:PULM:PERiod <value> [:SOURce<ch>]:PULM:PERiod?
EQUIVALENT MENU	Analog Mod > PULSE > Pulse Period
EXAMPLE	<i>:SOURce1:PULM:INT1:PERiod 900 ns</i> <i>:SOURce1:PULM:INT1:PERiod?</i> Return: <i>9e-07\n</i>

3.4.8.3.6 Pulse Width ([:SOURce<ch>]:PULM:WIDTH)

SYNTAX	[:SOURce<ch>]:PULM:WIDTH <value> [:SOURce<ch>]:PULM:WIDTH?
DESCRIPTION	When the pulse mode of the specified channel is Single, this command sets/queries the pulse width; when the pulse mode of the specified channel is Double, this command sets/queries the pulse width of the first pulse.
DATA TYPE	Float, unit: ns, us, ms or s, default is s
RANGE	20 ns ~ 300 s
RETURN	Float, unit: s
DEFAULT VALUE	2 ms
EQUIVALENT SCPI	[:SOURce<ch>]:PULM:INT[1<ch>]:PWIDTH <value> [:SOURce<ch>]:PULM:INT[1<ch>]:PWIDTH?
EQUIVALENT MENU	Analog Mod > PULSE > Pulse Width
EXAMPLE	<i>:SOURce1:PULM:WIDT 33 us</i> <i>:SOURce1:PULM:WIDT?</i> Return: <i>3.3e-05\n</i>

3.4.8.3.7 Pulse Width ([:SOURce<ch>]:PULM:INT[1]:PWIDth)

SYNTAX	[:SOURce<ch>]:PULM:INT[1]:PWIDth <value> [:SOURce<ch>]:PULM:INT[1]:PWIDth?
DESCRIPTION	When the pulse mode of the specified channel is Single, this command sets/queries the pulse width; when the pulse mode of the specified channel is Double, this command sets/queries the pulse width of the first pulse.
DATA TYPE	Float, unit: ns, us, ms or s, default is s
RANGE	20 ns ~ 300 s
RETURN	Float, unit: s
DEFAULT VALUE	2 ms
EQUIVALENT SCPI	[:SOURce<ch>]:PULM:WIDTh <value> [:SOURce<ch>]:PULM:WIDTh?
EQUIVALENT MENU	Analog Mod > PULSE > Pulse Width
EXAMPLE	<i>:SOURce1:PULM:INT:PWIDth 400 ns</i> <i>:SOURce1:PULM:INT:PWIDth?</i> Return: <i>4e-07\n</i>

3.4.8.3.8 Double Pulse Delay ([:SOURce<ch>]:PULM:DOUBle:DELaY)

SYNTAX	[:SOURce<ch>]:PULM:DOUBle:DELaY <value> [:SOURce<ch>]:PULM:DOUBle:DELaY?
DESCRIPTION	When the pulse mode of the specified channel is Double, this command sets/queries the double pulse delay.
DATA TYPE	Float, unit: ns, us, ms or s, default is s
RANGE	20 ns ~ 300 s
RETURN	Float, unit: s
DEFAULT VALUE	4 ms
EQUIVALENT MENU	Analog Mod > PULSE > Double Pulse Delay
EXAMPLE	<i>:SOURce1:PULM:DOUBle:DELaY 2 ms</i> <i>:SOURce1:PULM:DOUBle:DELaY?</i> Return: <i>0.002\n</i>

3.4.8.3.9 #2 Width ([:SOURce<ch>]:PULM:DOUBle:WIDTh)

SYNTAX	[:SOURce<ch>]:PULM:DOUBle:WIDTh <time> [:SOURce<ch>]:PULM:DOUBle:WIDTh?
DESCRIPTION	When the pulse mode of the specified channel is Double, this command sets/queries the pulse width of the second pulse.
DATA TYPE	Float, unit: ns, us, ms or s, default is s
RANGE	20 ns ~ 300 s
RETURN	Float, unit: s
DEFAULT VALUE	2 ms
EQUIVALENT MENU	Analog Mod > PULSE > #2 Width
EXAMPLE	<i>:SOURce1:PULM:DOUBle:WIDTh 5 ms</i> <i>:SOURce1:PULM:DOUBle:WIDTh?</i> Return: <i>0.005\n</i>

3.4.8.3.10 Pulse Train Add Row ([:SOURce<ch>]:PULM:TRAI:n:PAIR)

SYNTAX	[:SOURce<ch>]:PULM:TRAI:n:PAIR <row>
DESCRIPTION	This command copies the specified line and pastes it before the specified line in the pulse train of the specified channel.
DATA TYPE	Integer
RANGE	1 ~ total number of rows in the pulse train
EQUIVALENT MENU	Analog Mod > PULSE > Pulse Train > Add
EXAMPLE	<i>PULM:TRAI:n:PAIR 1</i>

3.4.8.3.11 Pulse Train Delete Row ([:SOURce<ch>]:PULM:TRAI:n:DELeTe)

SYNTAX	[:SOURce<ch>]:PULM:TRAI:n:DELeTe <row>
DESCRIPTION	This command removes a specified row from the pulse train of the specified channel.
DATA TYPE	Integer
RANGE	1 ~ total number of rows in the pulse train
EQUIVALENT MENU	Analog Mod > PULSE > Pulse Train > Delete
EXAMPLE	<i>:SOURce1:PULM:TRAI:n:DELeTe 5</i>

3.4.8.3.12 Pulse Train Edit On Time ([:SOURce<ch>]:PULM:TRAI:n:DATA:ONTIme)

SYNTAX	[:SOURce<ch>]:PULM:TRAI:n:DATA:ONTIme <raw>,<on_time>
DESCRIPTION	This command edits the positive pulse width of the specified row in the pulse train of the specified channel.
DATA TYPE	Row: Integer, On_time: float, unit: ns, us, ms or s, default is s
RANGE	Row: 1 ~ total number of rows in the pulse train, On_time: 20 ns ~ 300 s
EQUIVALENT MENU	Analog Mod > PULSE > Pulse Train
EXAMPLE	<i>[:SOURce1:PULM:TRAI:n:DATA:ONTIme 1,10 ms]</i>

3.4.8.3.13 Pulse Train Edit Off Time ([:SOURce<ch>]:PULM:TRAI:n:DATA:OFFTime)

SYNTAX	[:SOURce<ch>]:PULM:TRAI:n:DATA:OFFTime <raw>,<off_time>
DESCRIPTION	This command edits the negative pulse width of the specified row in the pulse train of the specified channel.
DATA TYPE	Row: Integer, Off_time: float, unit: ns, us, ms or s, default is s
RANGE	Row: 1 ~ total number of rows in the pulse train, Off_time: 20 ns ~ 300 s
EQUIVALENT MENU	Analog Mod > PULSE > Pulse Train
EXAMPLE	<i>[:SOURce1:PULM:TRAI:n:DATA:OFFTime 1, 20 ms]</i>

3.4.8.3.14 Pulse Train Edit Count ([:SOURce<ch>]:PULM:TRAI:n:DATA:COUNt)

SYNTAX	[:SOURce<ch>]:PULM:TRAI:n:DATA:COUNt <raw>,<count>
DESCRIPTION	This command edits the number of repetitions for a specified row of the pulse train of the specified channel.
DATA TYPE	Row: integer, Count: integer
RANGE	Row: 1 ~ total number of rows in the pulse train, Count: 1 ~ 65535
EQUIVALENT MENU	Analog Mod > PULSE > Pulse Train
EXAMPLE	<i>[:SOURce1:PULM:TRAI:n:DATA:COUNt 1,3]</i>

3.4.8.3.15 Pulse Train Edit ([:SOURce<ch>]:PULM:TRAI:CHANGe)

SYNTAX	[:SOURce<ch>]:PULM:TRAI:CHANGe <row>,<on_time>,<off_time>,<count>
DESCRIPTION	This command edits the specified row of the pulse train of the specified channel.
DATA TYPE	Row: integer, On_time: float, unit: ns, us, ms or s, default is s, Off_time: float, unit: ns, us, ms or s, default is s, Count: integer
RANGE	Row: 1 ~ total number of rows in the pulse train, On_time: 20 ns ~ 300 s, Off_time: 20 ns ~ 300 s, Count: 1 ~ 65535
EQUIVALENT MENU	Analog Mod > PULSE > Pulse Train
EXAMPLE	<i>:SOURce1:PULM:TRAI:CHANGe 2,3 ms,500 ns,4</i>

3.4.8.3.16 Pulse Train Data ([:SOURce<ch>]:PULM:TRAI:LIST?)

SYNTAX	[:SOURce<ch>]:PULM:TRAI:LIST? <begin_row>,<end_row>
DESCRIPTION	This command queries the data from begin_row to end_row in the pulse train of the specified channel.
DATA TYPE	Integer, Integer
RANGE	1 ~ total number of rows in the pulse train, Start row ~ total number of rows in the pulse train
RETURN	String
EQUIVALENT MENU	Analog Mod > PULSE > Pulse Train
EXAMPLE	<i>:SOURce1:PULM:TRAI:LIST? 1,3</i> Return: <i>0.001,0.005,1\0.003,0.003,2\0.004,0.002,1\n</i>

3.4.8.3.17 Pulse Train Count ([:SOURce<ch>]:PULM:TRAI:COUNT?)

SYNTAX	[:SOURce<ch>]:PULM:TRAI:COUNT?
DESCRIPTION	This command queries the number of rows in the pulse train of the specified channel.

EQUIVALENT MENU	Analog Mod > PULSE > Pulse Train
EXAMPLE	<i>:SOURce1:PULM:TRAI:n:COUNt?</i> Return: <i>5ln</i>

3.4.8.3.18 Pulse Train Clear ([[:SOURce<ch>]:PULM:TRAI:n:CLEAR])

SYNTAX	[[:SOURce<ch>]:PULM:TRAI:n:CLEAR]
DESCRIPTION	This command clears the pulse train of the specified channel and restores its default value.
EQUIVALENT MENU	Analog Mod > PULSE > Pulse Train > Clear
EXAMPLE	<i>:SOURce1:PULM:TRAI:n:CLEAR</i>

3.4.8.3.19 Pulse Train Load ([[:SOURce<ch>]:PULM:TRAI:n:LOAD])

SYNTAX	[[:SOURce<ch>]:PULM:TRAI:n:LOAD <"file_name">]
DESCRIPTION	This command loads the pulse train of the specified channel from the file.
DATA TYPE	String
RANGE	None
EQUIVALENT MENU	Analog Mod > PULSE > Pulse Train > Load
EXAMPLE	<i>:SOURce1:PULM:TRAI:n:LOAD "U-disk3/test.pulstrn"</i>

3.4.8.3.20 Pulse Train Store ([[:SOURce<ch>]:PULM:TRAI:n:STORE])

SYNTAX	[[:SOURce<ch>]:PULM:TRAI:n:STORE <"file_name">]
DESCRIPTION	This command saves the pulse train of the specified channel into file.
DATA TYPE	String
RANGE	None
EQUIVALENT MENU	Analog Mod > PULSE > Pulse Train > Save
EXAMPLE	<i>:SOURce1:PULM:TRAI:n:STORE "test.pulstrn"</i> <i>:SOURce1:PULM:TRAI:n:STORE "U-disk1/test.pulstrn"</i>

3.4.8.3.21 Trigger Out ([[:SOURce<ch>]:PULM:TRIGger:STATe])

SYNTAX	[[:SOURce<ch>]:PULM:TRIGger:STATe ON OFF 1 0 [:SOURce<ch>]:PULM:TRIGger:STATe?
DESCRIPTION	This command sets/gets the pulse trigger output status of the specified channel.
DATA TYPE	Boolean
RANGE	ON OFF 1 0
RETURN	1 0
DEFAULT VALUE	1
EQUIVALENT MENU	Analog Mod > PULSE > Trigger Out
EXAMPLE	<i>:SOURce1:PULM:TRIGger:STATe OFF</i> <i>:SOURce1:PULM:TRIGger:STATe?</i> Return: <i>0\n</i>

3.4.8.3.22 Pulse Trigger ([[:SOURce<ch>]:PULM:TRIGger:MODE])

SYNTAX	[[:SOURce<ch>]:PULM:TRIGger:MODE AUTO KEY EXTErnal EGATe [:SOURce<ch>]:PULM:TRIGger:MODE?
DESCRIPTION	This command sets/queries the pulse trigger mode of the specified channel.
DATA TYPE	Enumeration
RANGE	AUTO KEY EXTErnal EGATe
RETURN	Enumeration
DEFAULT VALUE	AUTO
EQUIVALENT MENU	Analog Mod > PULSE > Pulse Trigger
EXAMPLE	<i>:SOURce1:PULM:TRIG:MODE EXTErnal</i> <i>:SOURce1:PULM:TRIGger:MODE?</i> Return: <i>EXTErnal\n</i>

3.4.8.3.23 Trigger Delay ([[:SOURce<ch>]:PULM:DELay])

SYNTAX	[[:SOURce<ch>]:PULM:DELay <value> [:SOURce<ch>]:PULM:DELay?
--------	--

DESCRIPTION	When the pulse trigger mode of the specified channel is EXTERNAL, this command sets/queries the trigger delay.
DATA TYPE	Float, unit: ns, us, ms or s, default is s
RANGE	140 ns ~ 300 s
RETURN	Float, unit: s
DEFAULT VALUE	140 ns
EQUIVALENT MENU	Analog Mod > PULSE > Trig Delay
EXAMPLE	<i>:SOURce1:PULM:DEL 30 ms</i> <i>:SOURce1:PULM:DELAy?</i> Return: <i>0.031n</i>

3.4.8.3.24 Trigger Slope ([SOURce<ch>]:PULM:TRIGger:EXternal:SLOPe)

SYNTAX	[SOURce<ch>]:PULM:TRIGger:EXternal:SLOPe NEGativePOSitive [SOURce<ch>]:PULM:TRIGger:EXternal:SLOPe?
DESCRIPTION	When the pulse trigger mode of the specified channel is EXTERNAL, this command sets/queries the trigger edge of the external trigger.
DATA TYPE	Enumeration
RANGE	NEGativePOSitive
RETURN	Enumeration
DEFAULT VALUE	POSitive
EQUIVALENT MENU	Analog Mod > PULSE > Trigger Slope
EXAMPLE	<i>:SOURce1:PULM:TRIG:EXT:SLOP NEG</i> <i>:SOURce1:PULM:TRIG:EXT:SLOP?</i> Return: <i>NEGative1n</i>


3.4.8.3.25 Trigger Polarity ([SOURce<ch>]:PULM:TRIGger:EXternal:GATE:POLarity)

SYNTAX	[SOURce<ch>]:PULM:TRIGger:EXternal:GATE:POLarity NORMallINverted [SOURce<ch>]:PULM:TRIGger:EXternal:GATE:POLarity?
DESCRIPTION	This command sets/queries the trigger polarity of the external trigger gating for pulse function of the specified channel.

DATA TYPE	Enumeration
RANGE	NORMal INVerted
RETURN	Enumeration
DEFAULT VALUE	NORMal
EQUIVALENT MENU	Analog Mod > PULSE > Trig Polarity
EXAMPLE	<pre><i>:SOURce1:PULM:TRIG:EXT:GATE:POL INVerted</i></pre> <pre><i>:SOURce1:PULM:TRIGger:EXternal:GATE:POLarity?</i></pre> Return: <pre><i>INVerted\n</i></pre>

3.4.9 Phase Coherence

3.4.9.1 Phase Coherence ([[:SOURce]:PHASe:COHerent])

SYNTAX	<pre>[[:SOURce]:PHASe:COHerent ON OFF 1 0</pre> <pre>[[:SOURce]:PHASe:COHerent?</pre>
DESCRIPTION	This command sets/queries the phase coherence function status of RF channel.
DATA TYPE	Boolean
RANGE	ON OFF 1 0
RETURN	ON OFF 1 0
DEFAULT VALUE	0
EQUIVALENT MENU	
EXAMPLE	<pre><i>:SOURce:PHASe:COHerent 1</i></pre> <pre><i>:SOURce:PHASe:COHerent?</i></pre> Return: <pre><i>1\n</i></pre>

3.4.9.2 Coherent Channel ([[:SOURce<ch>]:PHASe:COHerent:CHANnel])

SYNTAX	<pre>[[:SOURce<ch>]:PHASe:COHerent:CHANnel ON OFF 1 0</pre> <pre>[[:SOURce<ch>]:PHASe:COHerent:CHANnel?</pre>
DESCRIPTION	When phase coherence status is on, this command sets/queries whether the phase of RF Channel ch is coherent with other channels.

DATA TYPE	Boolean
RANGE	ON OFF 1 0
RETURN	ON OFF 1 0
DEFAULT VALUE	0
EQUIVALENT MENU	 >  > 
EXAMPLE	<pre><i>:SOURce1:PHASe:COHerent:CHANnel 1</i> <i>:SOURce1:PHASe:COHerent:CHANne?</i></pre> Return: <pre><i>1\n</i></pre>

3.4.9.3 Coherent Frequency ([[:SOURce]:PHASe:COHerent: FREQuency])

SYNTAX	<pre>[[:SOURce]:PHASe:COHerent:FREQuency 22E9 [:SOURce]:PHASe:COHerent:FREQuency?</pre>
DESCRIPTION	When phase coherence status is on, all channels must use the same frequency. This command sets/queries the common frequency used for synchronizing all channels.
DATA TYPE	Float
RANGE	Minimum RF frequency ~ Maximum RF frequency
RETURN	Set frequency
DEFAULT VALUE	22000000000
EQUIVALENT MENU	 >  > 
EXAMPLE	<pre><i>:SOURce:PHASe:COHerent:FREQuency 22E9</i> <i>:SOURce:PHASe:COHerent:FREQuency?</i></pre> Return: <pre><i>22000000000\n</i></pre>

3.4.9.4 Frequency Synchronization([[:SOURce]:PHASe:COHerent:SYNC:FREQuency])

SYNTAX	<pre>:SOURce:PHASe:COHerent:SYNC:FREQuency</pre>
DESCRIPTION	This command synchronizes the frequency of phase-coherent channels to the configured phase-coherent frequency.
DATA TYPE	None

RANGE	None
RETURN	None
DEFAULT VALUE	None
EQUIVALENT MENU	 >  > 
EXAMPLE	<i>:PHase:COHerent:SYNC:FREQuency</i>

3.4.10 System Preset

3.4.10.1 Preset (:SOURce:PRESet)

SYNTAX	:SOURce:PRESet
DESCRIPTION	This command sets the instrument status to factory settings.
EQUIVALENT MENU	None
EXAMPLE	<i>:SOURce:PRESet</i>

3.5 SENSE Commands

3.5.1 Power Sensor

3.5.1.1 Sensor Info (:SENSe[:POWER]:TYPE?)

SYNTAX	:SENSe[:POWER]:TYPE?
DESCRIPTION	This command queries the model of the power sensor connected to the multi-channel microwave signal generator.
RETURN	String
DEFAULT VALUE	None
EQUIVALENT MENU	 >  >  > Sensor Info
EXAMPLE	<i>SENSe:TYPE?</i> Return: <i>NRP6A1n</i>

3.5.1.2 Sensor State (:SENSe[:POWer]:STATus)

SYNTAX	:SENSe[:POWer]:STATus OFF ON 0 1 :SENSe[:POWer]:STATus?
DESCRIPTION	This command sets/queries the measurement status of the power sensor.
DATA TYPE	Boolean
RANGE	ON OFF 1 0
RETURN	1 0
DEFAULT VALUE	0
EQUIVALENT MENU	 >  >  > Sensor State
EXAMPLE	<i>SENSe:STATus ON</i> <i>SENSe:STATus?</i> Return: <i>1\n</i>

3.5.1.3 Measurement (:SENSe[:POWer]:VALue?)


SYNTAX	:SENSe[:POWer]:VALue?
DESCRIPTION	This command queries the measured value of the power sensor.
RETURN	Float, unit: dBm
DEFAULT VALUE	None
EQUIVALENT MENU	 >  >  > Measurement
EXAMPLE	<i>SENSe:VALue?</i> Return: <i>-0.02600282\n</i>

3.5.1.4 Statistics State (:SENSe[:POWer]:STATistics:STATe)

SYNTAX	:SENSe[:POWer]:STATistics:STATe ON OFF 1 0 :SENSe[:POWer]:STATistics:STATe?
DESCRIPTION	This command sets/queries the measurement statistics status of the power sensor.
DATA TYPE	Boolean

RANGE	ON OFF 1 0
RETURN	1 0
DEFAULT VALUE	0
EQUIVALENT MENU	 >  >  > Statistics
EXAMPLE	<i>SENSe:STATISTICS:STATe ON</i> <i>SENSe:STATISTICS:STATe?</i> Return: <i>1\n</i>

3.5.1.5 Statistics Value (:READ[:POWER]?)


SYNTAX	:READ[:POWER]?
DESCRIPTION	This command queries the average and maximum values of the power sensor measurement statistics.
RETURN	String The string format: average,maximum Average: float, unit: dBm, Maximum: float, unit: dBm.
DEFAULT VALUE	None
EQUIVALENT MENU	 >  >  > Statistics > mean/max
EXAMPLE	<i>READ?</i> Return: <i>-0.05,-0.04\n</i>

3.5.1.6 Statistics Max Value (:SENSe[:POWER]:STATISTICS:MAX?)

SYNTAX	:SENSe[:POWER]:STATISTICS:MAX?
DESCRIPTION	This command queries the maximum value of the power sensor measurement statistics.
RETURN	Float, unit: dBm.
DEFAULT VALUE	None
EQUIVALENT MENU	 >  >  > Statistics > max

EXAMPLE *SENSe:STATIStics:MAX?*
 Return:
-0.03117205\n

3.5.1.7 Statistics Min Value (:SENSe[:POWer]:STATIStics:MIN?)

SYNTAX	:SENSe[:POWer]:STATIStics:MIN?
DESCRIPTION	This command queries the minimum value of the power sensor measurement statistics.
RETURN	Float, unit: dBm.
DEFAULT VALUE	None
EQUIVALENT MENU	 >  >  > Statistics > min
EXAMPLE	<i>SENSe:STATIStics:MIN?</i> Return: <i>-0.06101395\n</i>

3.5.1.8 Statistics Mean Value (:SENSe[:POWer]:STATIStics:AVG?)

SYNTAX	:SENSe[:POWer]:STATIStics:AVG?
DESCRIPTION	This command queries the average value of the power sensor measurement statistics.
RETURN	Float, unit: dBm.
DEFAULT VALUE	None
EQUIVALENT MENU	 >  >  > Statistics > mean
EXAMPLE	<i>SENSe:STATIStics:AVG?</i> Return: <i>-0.0322136383619456\n</i>

3.5.1.9 Statistics Count (:SENSe[:POWer]:STATIStics:COUNT?)

SYNTAX	:SENSe[:POWer]:STATIStics:COUNT?
DESCRIPTION	This command queries the count of the power sensor measurement statistics.

RETURN	Integer
DEFAULT VALUE	None
EQUIVALENT MENU	 >  >  > Statistics > count
EXAMPLE	<i>SENSe:STATISTICS:COUNt?</i> Return: <i>2035\n</i>

3.5.1.10 Statistics Clear (:SENSe[:POWer]:STATISTICS:CLEAr)

SYNTAX	:SENSe[:POWer]:STATISTICS:CLEAr
DESCRIPTION	This command clears the measurement statistics of the power sensor.
EQUIVALENT MENU	 >  >  > Statistics > clear
EXAMPLE	<i>SENSe:STATISTICS:CLEAr</i>

3.5.1.11 Level Control (:SENSe[:POWer]:LEV:CTL:STATe)

SYNTAX	:SENSe[:POWer]:LEV:CTL:STATe ON OFF 1 0 :SENSe[:POWer]:LEV:CTL:STATe?
DESCRIPTION	This command sets/queries the level control state of the power sensor.
DATA TYPE	Boolean
RANGE	ON OFF 1 0
RETURN	1 0
DEFAULT VALUE	0
EQUIVALENT SCPI	[:SOURce]:POWer:SPC:STATe ON OFF 1 0 [:SOURce]:POWer:SPC:STATe?
EQUIVALENT MENU	 >  >  > Level Control
EXAMPLE	<i>:SENSe:LEV:CTL:STATe OFF</i> <i>:SENSe:LEV:CTL:STATe?</i> Return: <i>0\n</i>

3.5.1.12 Target Level (:SENSe[:POWer]:SPC:TARGet)


SYNTAX	:SENSe[:POWer]:SPC:TARGet <power> :SENSe[:POWer]:SPC:TARGet?
DESCRIPTION	This command sets/queries the target level of the power sensor level control.
DATA TYPE	Float, unit: dBm, dBuV, uV, mV, V, nW, uW, mW or W, default is dBm
RANGE	-120 dBm ~ 20 dBm
RETURN	Float, unit: dBm
DEFAULT VALUE	0
EQUIVALENT SCPI	[:SOURce]:POWer:SPC:TARGet <power> [:SOURce]:POWer:SPC:TARGet?
EQUIVALENT MENU	 >  >  > Level Control > Target Level
EXAMPLE	<i>SENSe:SPC:TARGet -6</i> <i>SENSe:SPC:TARGet?</i> Return: <i>-6ln</i>

3.5.1.13 Channel Selection (:SENSe[:POWer]:LOGGing:STATe)

SYNTAX	:SENSe[:POWer]:LEV:CTL:CHANnel :SENSe[:POWer]:LEV:CTL:CHANnel? [:SOURce]:POWer:LEV:CTL:CHANnel [:SOURce]:POWer:LEV:CTL:CHANnel?
DESCRIPTION	This command sets/queries the channel of the power sensor level control.
DATA TYPE	Integer
RANGE	Dual-channel: 1 2, Four-channel: 1 2 3 4
RETURN	1 0
DEFAULT VALUE	0
EQUIVALENT SCPI	[:SOURce]:POWer:SPC:TARGet <power> [:SOURce]:POWer:SPC:TARGet?
EQUIVALENT MENU	 >  >  > Logging

EXAMPLE *:SENSe[:POWer]:LEV:CTL:CHANnel 1*
 :SENSe[:POWer]:LEV:CTL:CHANnel?
 Return:
 1\n

3.5.1.14 Limit Level (:SENSe[:POWer]:LIMit)

SYNTAX	:SENSe[:POWer]:LIMit <power> :SENSe[:POWer]:LIMit?
DESCRIPTION	This command sets/queries the Limit level of the power sensor level control.
DATA TYPE	Float, unit: dBm, dBuV, uV, mV, V, nW, uW, mW or W, default is dBm
RANGE	-120 dBm ~ 20 dBm
RETURN	Float, unit: dBm
DEFAULT VALUE	0
EQUIVALENT SCPI	[[:SOURce]:POWer:LIMit <power> [:SOURce]:POWer:LIMit?
EQUIVALENT MENU	HOME >  >  > Level Control > Limit Level
EXAMPLE	<i>SENSe:LIMit 2</i> <i>SENSe:LIMit?</i> Return: <i>2\n</i>

3.5.1.15 Catch Range (:SENSe[:POWer]:SPC:CRANge)

SYNTAX	:SENSe[:POWer]:SPC:CRANge <power> :SENSe[:POWer]:SPC:CRANge?
DESCRIPTION	This command sets/queries the catch range of the power sensor level control.
DATA TYPE	Float, unit: dB
RANGE	0 ~ 50
RETURN	Float, unit: dB
DEFAULT VALUE	0
EQUIVALENT SCPI	[[:SOURce]:POWer:SPC:CRANge <power>

[SOURce]:POWer:SPC:CRANge?

EQUIVALENT MENU

 >  >  > Level Control > Catch Range

EXAMPLE

*:SENSe:SPC:CRANge 10**:SENSe:SPC:CRANge?*

Return:

10\n

3.5.1.16 Auto Zero (:CALibration:ZERO:TYPE)

SYNTAX

:CALibration:ZERO:TYPE INTernal|EXTernal
:CALibration:ZERO:TYPE?

DESCRIPTION

This command sets/queries the automatic zero adjustment type of the power sensor.

DATA TYPE

Enumeration

RANGE

INTernal|EXTernal

RETURN

Enumeration

DEFAULT VALUE

INTernal

EQUIVALENT MENU

 >  >  > Auto Zero

EXAMPLE

*:CALibration:ZERO:TYPE EXTernal**:CALibration:ZERO:TYPE?*

Return:

EXTernal\n

3.5.1.17 Zeroing (:SENSe[:POWer]:ZERO)

SYNTAX

:SENSe[:POWer]:ZERO

DESCRIPTION

This command performs a zeroing operation on the power sensor.

EQUIVALENT MENU

 >  >  > Click to perform zeroing

EXAMPLE

:SENSe:ZERO

3.5.1.18 Frequency Type (:SENSe[:POWer]:SOURce)

SYNTAX	:SENSe[:POWer]:SOURce RFIUSER :SENSe[:POWer]:SOURce?
DESCRIPTION	This command sets/queries the measurement frequency type of the power sensor.
DATA TYPE	Enumeration
RANGE	RFIUSER
RETURN	Enumeration
DEFAULT VALUE	RF
EQUIVALENT MENU	 >  >  > Frequency
EXAMPLE	<i>SENSe:SOURce USER</i> <i>SENSe:SOURce?</i> Return: <i>USER\n</i>

3.5.1.19 Frequency (:SENSe[:POWer]:FREQuency)

SYNTAX	:SENSe[:POWer]:FREQuency <freq> :SENSe[:POWer]:FREQuency?
DESCRIPTION	This command sets/queries the manual measurement frequency of the power sensor.
DATA TYPE	Float, unit: Hz, kHz, MHz or GHz, default is Hz
RANGE	Power sensor measurement range
RETURN	Float, unit: Hz
DEFAULT VALUE	None
EQUIVALENT MENU	 >  >  > Frequency
EXAMPLE	<i>SENSe:FREQuency 1 MHz</i> <i>SENSe:FREQuency?</i> Return: <i>1000000\n</i>

3.5.1.20 Level Offset State (:SENSe[:POWer]:OFFSet:STATe)

SYNTAX	:SENSe[:POWer]:OFFSet:STATe ON OFF 1 0 :SENSe[:POWer]:OFFSet:STATe?
DESCRIPTION	This command sets/queries the level offset state of the power sensor.
DATA TYPE	Boolean
RANGE	ON OFF 1 0
RETURN	1 0
DEFAULT VALUE	0
EQUIVALENT MENU	 >  >  > Level Offset
EXAMPLE	<i>SENSe:OFFSet:STATe ON</i> <i>SENSe:OFFSet:STATe?</i> Return: <i>1\n</i>

3.5.1.21 Level Offset (:SENSe[:POWer]:OFFSet)

SYNTAX	:SENSe[:POWer]:OFFSet <power> :SENSe[:POWer]:OFFSet?
DESCRIPTION	This command sets/queries the level offset value of the power sensor.
DATA TYPE	Float, unit: dB
RANGE	-200 ~ 200
RETURN	Float, unit: dB
DEFAULT VALUE	0
EQUIVALENT MENU	 >  >  > Level Offset
EXAMPLE	<i>SENSe:OFFSet 10</i> <i>SENSe:OFFSet?</i> Return: <i>10\n</i>

3.5.1.22 Average Type (:SENSe[:POWer]:FILTer:TYPE)

SYNTAX	:SENSe[:POWer]:FILTer:TYPE AUTO USER NSRatio :SENSe[:POWer]:FILTer:TYPE?
DESCRIPTION	This command sets/queries the measurement averaging type of the power sensor.
DATA TYPE	Enumeration
RANGE	AUTO USER NSRatio
RETURN	Enumeration
DEFAULT VALUE	AUTO
EQUIVALENT MENU	 >  >  > Averaging
EXAMPLE	<i>SENSe:FILTer:TYPE USER</i> <i>SENSe:FILTer:TYPE?</i> Return: <i>USER\n</i>

3.5.1.23 Average Times (:SENSe[:POWer]:FILTer:LENGth)

SYNTAX	:SENSe[:POWer]:FILTer:LENGth <length> :SENSe[:POWer]:FILTer:LENGth?
DESCRIPTION	This command sets/queries the average number of measurements of the power sensor.
DATA TYPE	Integer
RANGE	1 ~ 65536
RETURN	Integer
DEFAULT VALUE	None
EQUIVALENT MENU	 >  >  > Averaging Count
EXAMPLE	<i>SENSe:FILTer:LENGth 10</i> <i>SENSe:FILTer:LENGth?</i> Return: <i>10\n</i>

3.5.1.24 Internal Noise (:SENSe[:POWer]:FILTer:NSRatio)

SYNTAX	:SENSe[:POWer]:FILTer:NSRatio <noise> :SENSe[:POWer]:FILTer:NSRatio?
DESCRIPTION	When the measurement averaging type of the power sensor is fixed noise, this command sets/queries the fixed noise of the power sensor.
DATA TYPE	Float, unit: dB
RANGE	None
RETURN	Float, unit: dB
DEFAULT VALUE	None
EQUIVALENT MENU	 >  >  > Internal Noise
EXAMPLE	<i>SENSe:FILTer:NSRatio 1</i> <i>SENSe:FILTer:NSRatio?</i> Return: <i>1ln</i>

3.5.1.25 Logging (:SENSe[:POWer]:LOGGing:STATe)

SYNTAX	:SENSe[:POWer]:LOGGing:STATe ON OFF 1 0 :SENSe[:POWer]:LOGGing:STATe?
DESCRIPTION	This command sets/queries the logging status of the power sensor.
DATA TYPE	Boolean
RANGE	ON OFF 1 0
RETURN	1 0
DEFAULT VALUE	0
EQUIVALENT MENU	 >  >  > Logging
EXAMPLE	<i>SENSe:LOGGing:STATe ON</i> <i>SENSe:LOGGing:STATe?</i> Return: <i>1ln</i>

4 Programming Examples

This chapter provides some examples for programmers. In these examples you can see how to use VISA or Sockets and the above SCPI commands to control a signal generator. By following these examples, you can develop more applications.

4.1 VISA Examples

4.1.1 VC++ Example

System environment: Windows 10, 64-bit operating system

Programming software: Visual Studio

Example content: Use NI-VISA to access and control the device through USBTMC or TCP/IP and perform read and write operations.

Please follow below steps to complete the example:

1. Open Visual Studio, and create a new VC++ win32 console project.
2. Set up the project environment to use the NI-VISA library. There are two ways to use the NI-VISA library, static or automatic:

(1) Static:


Find the files in the NI-VISA installation path: visa.h, visatype.h, visa32.lib. The default installation path of NI-VISA is "C:\Program Files\IVI Foundation\VISA\Win64\". Copy the above files into your project and add them to the project. Then add the following two lines of code in the project.cpp file:

```
#include "visa.h"
```


```
#pragma comment(lib,"visa32.lib")
```

(2) Automatic:


Set the include directory for header files. The default installation path of NI-VISA header files is "C:\Program Files\IVI Foundation\VISA\Win64\Include". Fill in the header file installation path in Project --- Properties --- C/C++ --- General --- Additional Include Directories, as shown below:

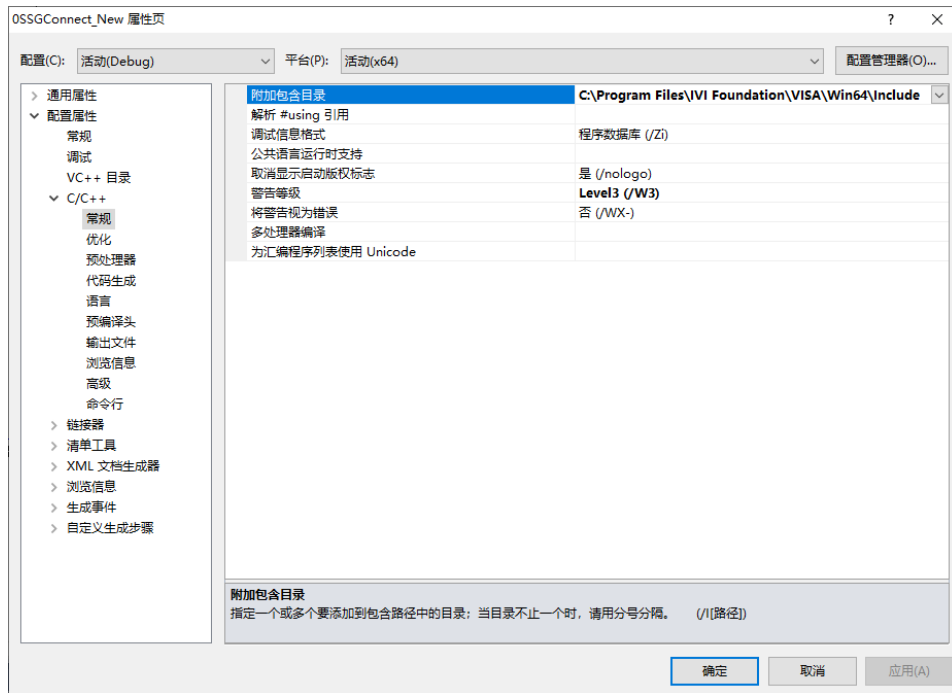

Set the include directory of library files. The default installation path of NI-VISA library files is “C:\Program Files\IVI Foundation\Visa\Win64\Lib_x64\msc”. Fill in the library file installation path in Project --- Properties --- Linker --- General --- Additional library directory, as shown below:

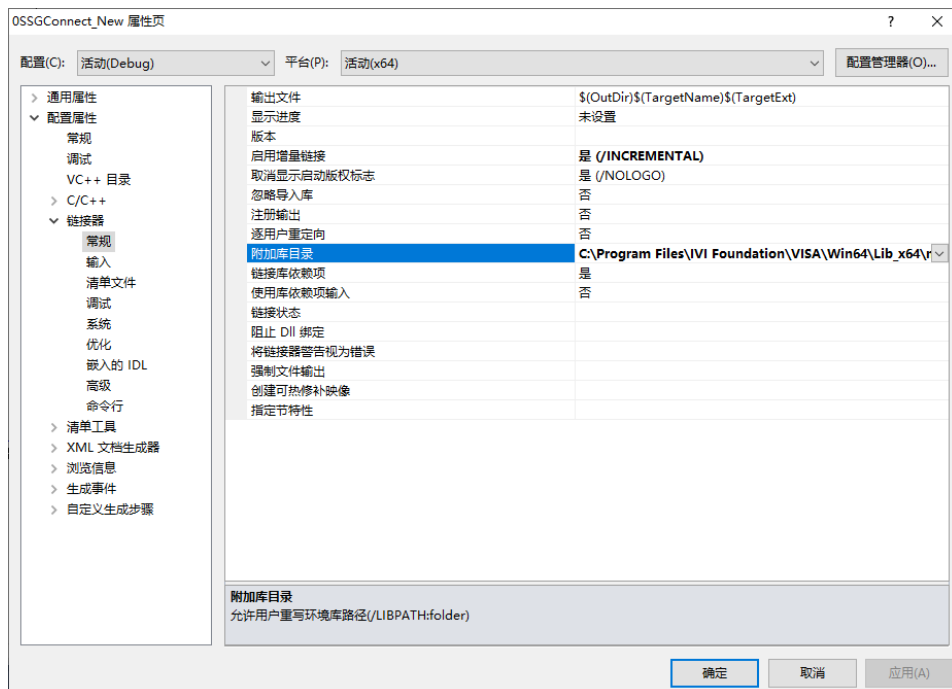

Set up library files. Fill in the library file name in Project --- Properties --- Linker --- Command Line --- Additional Options: visa32.lib, as shown below:

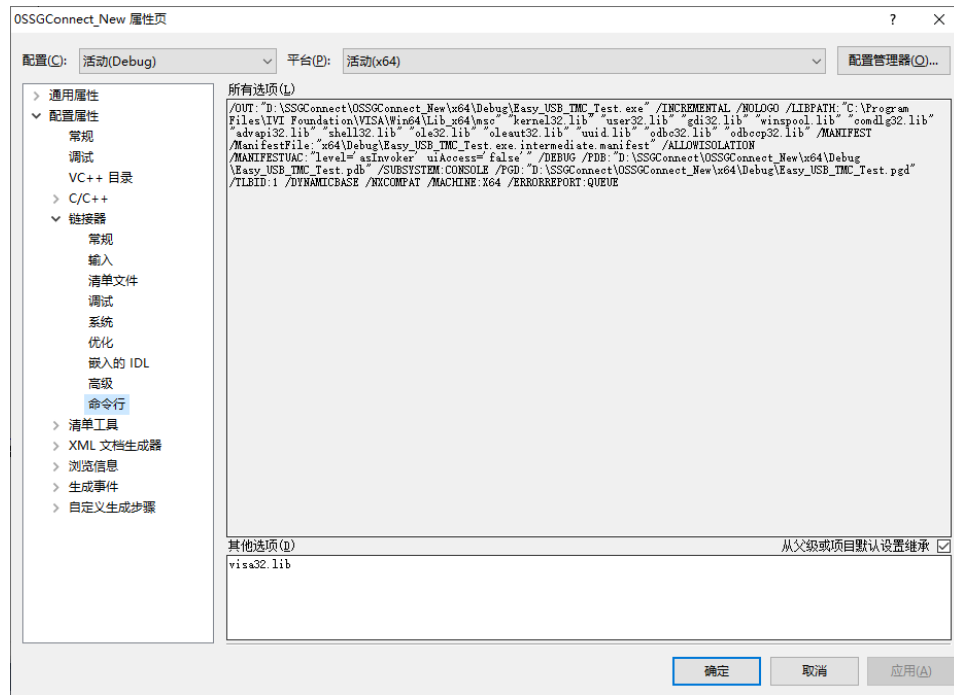

Finally, reference the header file in the project .cpp file:

```
#include <visa.h>
```

3. Add code

(1) USBTMC access code

Write a function Usbtmc_test:

```
int Usbtmc_test()
{
    /* This code demonstrates sending synchronous read & write commands */
    /* to an USB Test & Measurement Class (USBTMC) instrument using */
    /* NI-VISA */
    /* The example writes the "*IDN?\n" string to all the USBTMC */
    /* devices connected to the system and attempts to read back */
    /* results using the write and read functions. */
    /* The general flow of the code is */
    /* Open Resource Manager */
    /* Open VISA Session to an Instrument */
    /* Write the Identification Query Using viPrintf */
    /* Try to Read a Response With viScanf */
    /* Close the VISA Session */
    /*******/
    ViSession defaultRM;
    ViSession instr;
```

```
ViUInt32 numInstrs;
ViFindList findList;
ViStatus status;
char instrResourceString[VI_FIND_BUFLLEN];
unsigned char buffer[100];
int i;

/** First we must call viOpenDefaultRM to get the manager
 * handle. We will store this handle in defaultRM.*/
status = viOpenDefaultRM (&defaultRM);
if (status<VI_SUCCESS)
{
    printf ("Could not open a session to the VISA Resource Manager!\n");
    return status;
}

/* Find all the USB TMC VISA resources in our system and store the number of resources in the system in
numInstrs.*/
status = viFindRsrc (defaultRM, "USB?*INSTR", &findList, &numInstrs, instrResourceString);
if (status<VI_SUCCESS)
{
    printf ("An error occurred while finding resources.\nPress 'Enter' to continue.");
    fflush(stdin);
    getchar();
    viClose (defaultRM);
    return status;
}

/** Now we will open VISA sessions to all USB TMC instruments.
 * We must use the handle from viOpenDefaultRM and we must
 * also use a string that indicates which instrument to open. This
 * is called the instrument descriptor. The format for this string
 * can be found in the function panel by right clicking on the
 * descriptor parameter. After opening a session to the
 * device, we will get a handle to the instrument which we
 * will use in later VISA functions. The AccessMode and Timeout
 * parameters in this function are reserved for future
 * functionality. These two parameters are given the value VI_NULL.*/
for (i=0; i<int(numInstrs); i++)
{
    if (i> 0)
    {
        viFindNext (findList, instrResourceString);
    }
    status = viOpen (defaultRM, instrResourceString, VI_NULL, VI_NULL, &instr);
}
```

```

    if (status<VI_SUCCESS)
    {
        printf ("Cannot open a session to the device %d.\n", i+1);
        continue ;
    }

    /* * At this point we now have a session open to the USB TMC instrument.
    * We will now use the viPrintf function to send the device the string "*IDN?\n",
    * asking for the device's identification. */
    char * cmmmand = "*IDN?\n";
    status = viPrintf (instr, cmmmand);
    if (status<VI_SUCCESS)
    {
        printf ("Error writing to the device %d.\n", i+1);
        status = viClose (instr);
        continue;
    }

    /** Now we will attempt to read back a response from the device to
    * the identification query that was sent. We will use the viScanf
    * function to acquire the data.
    * After the data has been read the response is displayed. */
    status = viScanf(instr, "%t", buffer);
    if (status<VI_SUCCESS)
    {
        printf ("Error reading a response from the device %d.\n", i+1);
    }
    else
    {
        printf ("\nDevice %d: %s\n", i+1, buffer);
    }
    status = viClose (instr);
}


/** Now we will close the session to the instrument using
* viClose. This operation frees all system resources.      */
status = viClose (defaultRM);
printf("Press 'Enter' to exit.");
fflush(stdin);
getchar();
return 0;
}

int _tmain(int argc, _TCHAR* argv[])
{

```

```
    Usbtmc_test();  
    return 0;  
}
```

The running result:

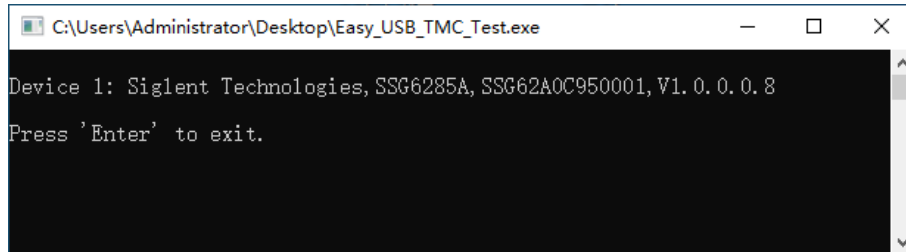

(2) TCP/IP access code

Write a function TCP_IP_Test:

```
int TCP_IP_Test(char *pIP)  
{  
    char outputBuffer[VI_FIND_BUFLLEN];  
    ViSession defaultRM, instr;  
    ViStatus status;  
  
    /* First we will need to open the default resource manager. */  
    status = viOpenDefaultRM (&defaultRM);  
    if (status<VI_SUCCESS)  
    {  
        printf("Could not open a session to the VISA Resource Manager!\n");  
    }  
  
    /* Now we will open a session via TCP/IP device */  
    char head[256] = "TCPIP0::";  
    char tail[] = "::INSTR";  
  
    strcat(head,pIP);  
    strcat(head,tail);  
    status = viOpen (defaultRM, head, VI_LOAD_CONFIG, VI_NULL, &instr);  
    if (status<VI_SUCCESS)  
    {  
        printf ("An error occurred opening the session\n");  
        viClose(defaultRM);  
    }  
    status = viPrintf(instr, "%idn?\n");  
    if (status<VI_SUCCESS)  
    {
```


```

        printf("Error writing to the device.\n");
        viClose(defaultRM);
    }
    status = viScanf(instr, "%t", outputBuffer);
    if (status<VI_SUCCESS)
    {
        printf("viRead failed with error code: %x \n",status);
        viClose(defaultRM);
    }
    else
    {
        printf ("\nMesseage read from device: %*s\n", 0,outputBuffer);
    }
    status = viClose (instr);
    status = viClose (defaultRM);
    printf("Press 'Enter' to exit.");
    fflush(stdin);
    getchar();
    return 0;
}

int _tmain(int argc, _TCHAR* argv[])
{
    printf("Please input IP address:");
    char ip[256];
    fflush(stdin);
    gets(ip);
    TCP_IP_Test(ip);
    return 0;
}

```

The running result:

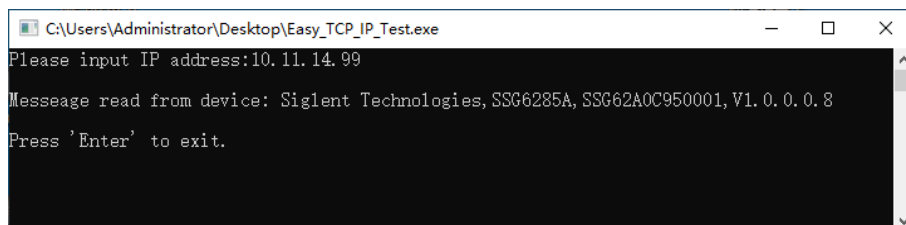

4.1.2 VB Example


System environment: Windows 7

Programming software: Microsoft Visual Basic 6.0

Example content: Use NI-VISA to access and control the device through USBTMC or TCP/IP and perform read and write operations.

Please follow below steps to complete the example:

1. Open Visual Basic and build a standard application program project (standard EXE).
2. Set up the project environment to use the NI-VISA library. Click the Existing tag of Project >> Add Existing Item, search for the visa32.bas file in the include folder under the NI-VISA installation path and add the file. This will enable VISA functions and VISA data types to be used in the program.

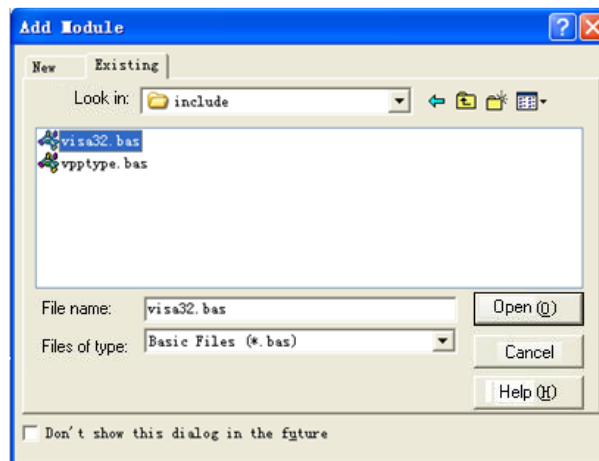

3. Add code
 - (1) USBTMC access code

Write a function Usbtmc_test:

Private Function Usbtmc_test() As Long

```
' This code demonstrates sending synchronous read & write commands
' to an USB Test & Measurement Class (USBTMC) instrument using
' NI-VISA
' The example writes the "*IDN?\n" string to all the USBTMC
' devices connected to the system and attempts to read back
' results using the write and read functions.
' The general flow of the code is
' Open Resource Manager
' Open VISA Session to an Instrument
' Write the Identification Query Using viWrite
```

```

' Try to Read a Response With viRead
' Close the VISA Session
Const MAX_CNT = 200

Dim defaultRM As Long
Dim instrsesn As Long
Dim numInstrs As Long
Dim findList As Long
Dim retCount As Long

Dim status As Long
Dim instrResourceString As String * VI_FIND_BUFLen
Dim Buffer As String * MAX_CNT
Dim i As Integer
' First we must call viOpenDefaultRM to get the manager
' handle. We will store this handle in defaultRM.
status = viOpenDefaultRM(defaultRM)
If (status < VI_SUCCESS) Then
    resultTxt.Text = "Could not open a session to the VISA Resource Manager!"
    Usbtmc_test = status
    Exit Function
End If

' Find all the USB TMC VISA resources in our system and store the
' number of resources in the system in numInstrs.
status = viFindRsrc(defaultRM, "USB?*INSTR", findList, numInstrs, instrResourceString)
If (status < VI_SUCCESS) Then
    resultTxt.Text = "An error occurred while finding resources."
    viClose(defaultRM)
    Usbtmc_test = status
    Exit Function
End If

' Now we will open VISA sessions to all USB TMC instruments.
' We must use the handle from viOpenDefaultRM and we must
' also use a string that indicates which instrument to open. This
' is called the instrument descriptor. The format for this string
' can be found in the function panel by right clicking on the
' descriptor parameter. After opening a session to the
' device, we will get a handle to the instrument which we
' will use in later VISA functions. The AccessMode and Timeout
' parameters in this function are reserved for future

```

' functionality. These two parameters are given the value VI_NULL.

For i = 0 To numInstrs

 If (i > 0) Then

 status = viFindNext(findList, instrResourceString)

 End If

 status = viOpen(defaultRM, instrResourceString, VI_NULL, VI_NULL, instrsesn)

 If (status < VI_SUCCESS) Then

 resultTxt.Text = "Cannot open a session to the device " + CStr(i + 1)

 GoTo NextFind

 End If

' At this point we now have a session open to the USB TMC instrument.

' We will now use the viWrite function to send the device the string "*IDN?",

' asking for the device's identification.

 status = viWrite(instrsesn, "*IDN?", 5, retCount)

 If (status < VI_SUCCESS) Then

 resultTxt.Text = "Error writing to the device."

 status = viClose(instrsesn)

 GoTo NextFind

 End If

' Now we will attempt to read back a response from the device to

' the identification query that was sent. We will use the viRead

' function to acquire the data.

' After the data has been read the response is displayed.

 status = viRead(instrsesn, Buffer, MAX_CNT, retCount)

 If (status < VI_SUCCESS) Then

 resultTxt.Text = "Error reading a response from the device." + CStr(i + 1)

 Else

 resultTxt.Text = "Read from device: " + CStr(i + 1) + " " + Buffer

 End If

 status = viClose(instrsesn)

Next i

' Now we will close the session to the instrument using

' viClose. This operation frees all system resources.

status = viClose(defaultRM)

Usbtmc_test = 0

End Function

(2) TCP/IP access code

Write a function TCP_IP_Test:

```
Private Function TCP_IP_Test(ByVal ip As String) As Long
    Dim outputBuffer As String * VI_FIND_BUFLen
    Dim defaultRM As Long
    Dim instrsesn As Long
    Dim status As Long
    Dim count As Long

    ' First we will need to open the default resource manager.
    status = viOpenDefaultRM(defaultRM)
    If (status < VI_SUCCESS) Then
        resultTxt.Text = "Could not open a session to the VISA Resource Manager!"
        TCP_IP_Test = status
        Exit Function
    End If

    ' Now we will open a session via TCP/IP device
    status = viOpen(defaultRM, "TCPIP0::" + ip + "::INSTR", VI_LOAD_CONFIG, VI_NULL, instrsesn)
    If (status < VI_SUCCESS) Then
        resultTxt.Text = "An error occurred opening the session"
        viClose(defaultRM)
        TCP_IP_Test = status
        Exit Function
    End If

    status = viWrite(instrsesn, "*IDN?", 5, count)
    If (status < VI_SUCCESS) Then
        resultTxt.Text = "Error writing to the device."
    End If

    status = viRead(instrsesn, outputBuffer, VI_FIND_BUFLen, count)
    If (status < VI_SUCCESS) Then
        resultTxt.Text = "Error reading a response from the device." + CStr(i + 1)
    Else
        resultTxt.Text = "read from device:" + outputBuffer
    End If



    status = viClose(instrsesn)
    status = viClose(defaultRM)
    TCP_IP_Test = 0

End Function
```

(3) Button control code:

```
Private Sub exitBtn_Click()  
    End  
End Sub  
Private Sub tcpipBtn_Click()  
    Dim stat As Long  
    stat = TCP_IP_Test(ipTxt.Text)  
    If (stat < VI_SUCCESS) Then  
        resultTxt.Text = Hex(stat)  
    End If  
End Sub  
Private Sub usbBtn_Click()  
    Dim stat As Long  
    stat = Usbtmc_test  
    If (stat < VI_SUCCESS) Then  
        resultTxt.Text = Hex(stat)  
    End If  
End Sub
```

The running result:

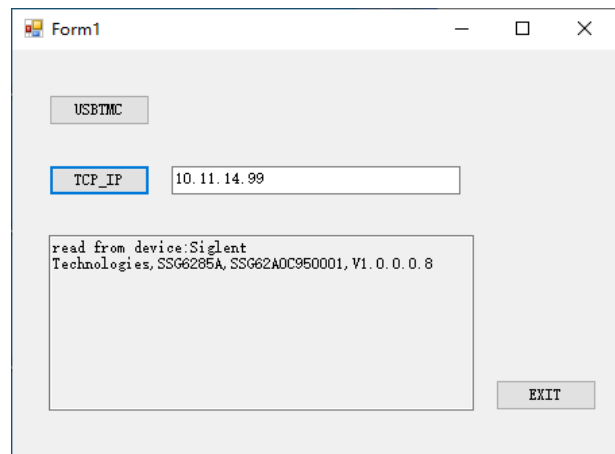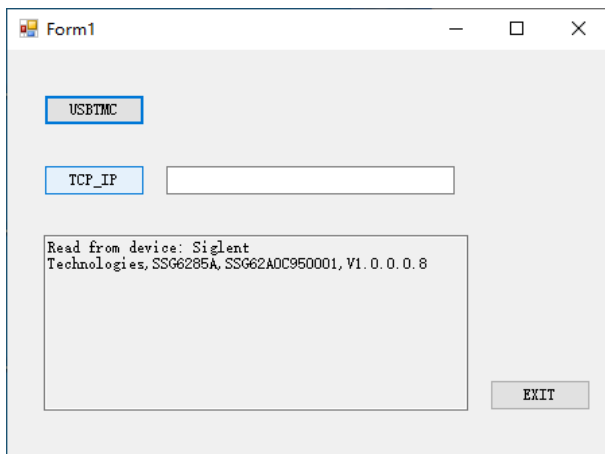

4.1.3 MATLAB Example

System environment: Windows 7

Programming software: MATLAB R2013a

Example content: Use NI-VISA to access and control the device through USBTMC or TCP/IP and perform read and write operations.

Please follow below steps to complete the example:

1. Open MATLAB and modify the current directory. In this example, change the current directory to D:\USBTMC_TCPIP_Demo.
2. Click File>>New>>Script in the MATLAB interface to create an empty M document.
3. Add code

(1) USBTMC access code

Write a function Usbtmc_test:

```
function USBTMC_test()
% This code demonstrates sending synchronous read & write commands
% to an USB Test & Measurement Class (USBTMC) instrument using
% NI-VISA

%Create a VISA-USB object connected to a USB instrument
vu = visa('ni','USB0::0xF4EC::0x1504::SSG6A_TESE0000::INSTR');

%Open the VISA object created
fopen(vu);


%Send the string "*IDN?",asking for the device's identification.
fprintf(vu,'*IDN?');

%Request the data
outputbuffer = fscanf(vu);
disp(outputbuffer);

%Close the VISA object
fclose(vu);
delete(vu);
clear vu;

end
```

The running result:

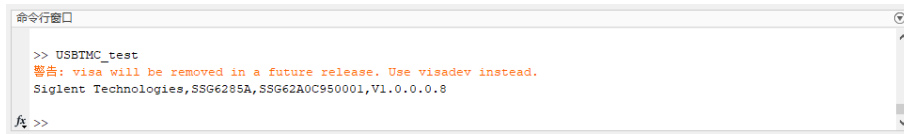

```

命令窗口
>> USBTMC_test
警告: visa will be removed in a future release. Use visadev instead.
Siglent Technologies,SSG6285A,SSG62A0C950001,V1.0.0.0.8
fx >>

```

(2) TCP/IP access code

Write a function TCP_IP_Test:

```

function TCP_IP_test()
% This code demonstrates sending synchronous read & write commands
% to an TCP/IP instrument using NI-VISA

%Create a VISA-TCPIP object connected to an instrument
%configured with IP address.
vt = visa('ni',[TCPIP0::','10.11.22.27','::INSTR']);

%Open the VISA object created
fopen(vt);

%Send the string "*IDN?",asking for the device's identification.
fprintf(vt, '*IDN?');


%Request the data
outputbuffer = fscanf(vt);
disp(outputbuffer);

%Close the VISA object
fclose(vt);
delete(vt);
clear vt;

end

```

The running result:

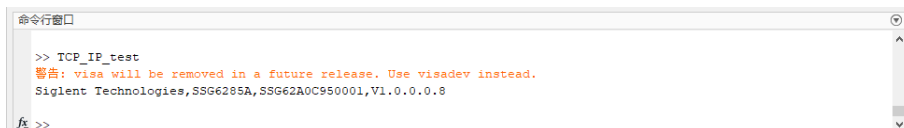

```

命令窗口
>> TCP_IP_test
警告: visa will be removed in a future release. Use visadev instead.
Siglent Technologies,SSG6285A,SSG62A0C950001,V1.0.0.0.8
fx >>

```

4.1.4 LabVIEW Example


System environment: Windows 7

Programming software: LabVIEW 2011


Example content: Use NI-VISA to access and control the device through USBTMC or TCP/IP and perform read and write operations.

Please follow below steps to complete the example:

1. Open LabVIEW and create a VI file.
2. Add controls. Right-click the front panel interface, select and add VISA resource name, error input, error out and some indicators in the controls column.
3. Open the block diagram interface. Right-click the VISA resource name and select from the shortcut menu of the VISA palette to add the following functions: VISA Write, VISA Read, VISA Open and VISA Close.
4. Connect them as shown in the figure below:

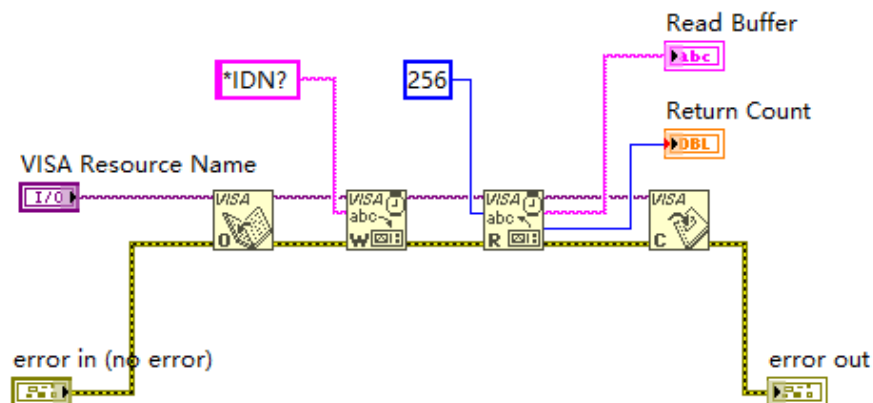


5. Select the device resource from the VISA resource name list box and run the program.

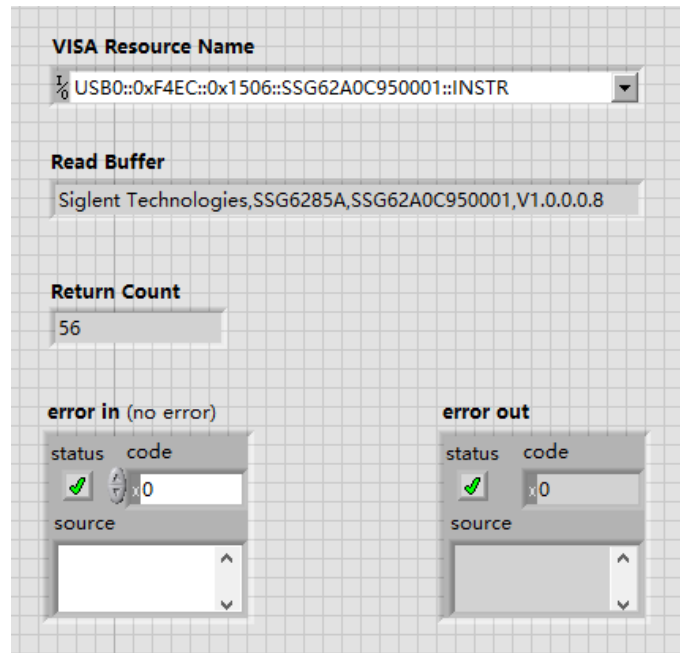

In this example, the VI opens a VISA session to the USBTMC device, writes a command to the device, and then reads back the response. In this example, the specific command sent is a device ID query. Please check the device command set with your device manufacturer. After all communication is complete, the VI closes the VISA session.

Communicating with the device over TCP/IP is similar to USBTMC. However, you need to change the VISA write and VISA read functions to synchronize the I/O. LabVIEW's default is asynchronous I/O. Right-click the node and select Synchronous I/O Mode>>Sync from the shortcut menu to write or read synchronized data.

1. Connect them as shown in the figure below:

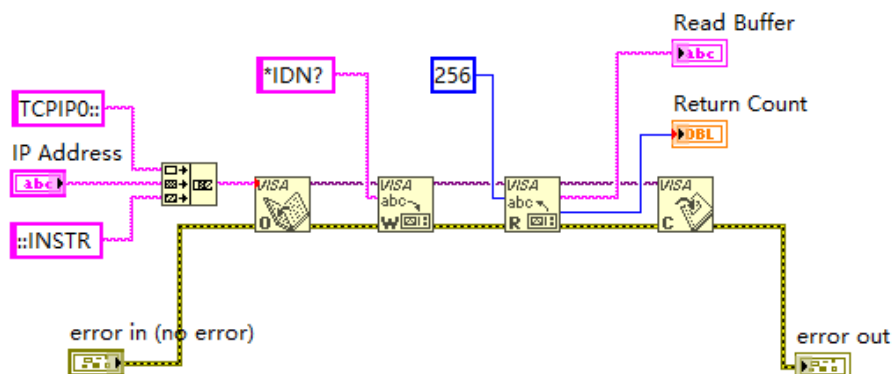

2. Enter the IP address and run the program:

IP Address	
10.11.14.99	
Read Buffer	
Siglent Technologies,SSG6285A,SSG62A0C950001,V1.0.0.0.8	
Return Count	
56	
error in (no error)	
status	code
	x0
source	
error out	
status	code
	x0
source	

4.2 Socket Examples

The Windows operating system itself supports Sockets communication, and this communication method is also relatively simple. It should be noted that "\n" (newline character) needs to be added to the end of the SCPI command string.

4.2.1 Python Example

Python is an interpreted programming language that allows you to work quickly and is very portable. Python has an underlying network module that provides access to the Socket interface, port 5025. Python scripts can be written for the Socket interface to perform various test and measurement tasks.

System environment: Windows 10, 64-bit operating system

Programming software: Python v3.6.5

Example content: Open a Socket, send a SCPI query, then close the Socket, loop ten times.

Below is the code of the script:

```
#!/usr/bin/env python
#-*- coding:utf-8 -*-
#-----
# The short script is an example that open a socket, sends a query,
# print the return message and closes the socket.
#-----
import socket    # for sockets
import sys      # for exit
import time     # for sleep
#-----
remote_ip = "10.11.22.27" # should match the instrument's IP address
port = 5025 # the port number of the instrument service

def SocketConnect():
    try:
        #create an AF_INET, STREAM socket (TCP)
        s = socket.socket(socket.AF_INET, socket.SOCK_STREAM)
    except socket.error:
        input('Failed to create socket. \nPress "Enter" to exit: ')
        sys.exit()
```

```

try:
    #Connect to remote server
    s.connect((remote_ip , port))
except socket.error:
    input('Failed to connect to ip %s!\nPress "Enter" to exit: ' % remote_ip)
    s.close()
    sys.exit()
return s

def SocketQuery(Sock, cmd):
    try :
        #Send cmd string
        Sock.sendall(cmd)
        time.sleep(1)
    except socket.error:
        #Send failed
        input('Send failed!\nPress "Enter" to exit: ')
        SocketClose(Sock)
        sys.exit()
    reply = Sock.recv(4096)
    reply = reply.decode()
    return reply

def SocketClose(Sock):
    #close the socket
    Sock.close()
    time.sleep(.300)

def main():
    # Body: send the SCPI commands *IDN? 10 times and print the return message
    s = SocketConnect()


    count = 0
    for i in range(10):
        qStr = SocketQuery(s, b'*IDN?\n')
        print (str(count) + ":: " + qStr)
        count = count + 1
    SocketClose(s)

```

```
input('Press "Enter" to exit')

if __name__ == '__main__':
    main()
```

The running result:

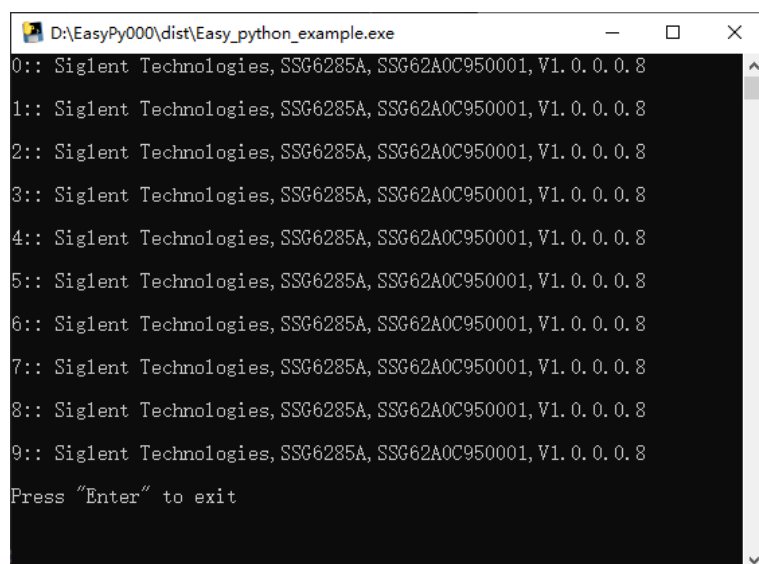

```
D:\EasyPy000\dist\Easy_python_example.exe
0:: Siglent Technologies, SSG6285A, SSG62A0C950001, V1.0.0.0.8
1:: Siglent Technologies, SSG6285A, SSG62A0C950001, V1.0.0.0.8
2:: Siglent Technologies, SSG6285A, SSG62A0C950001, V1.0.0.0.8
3:: Siglent Technologies, SSG6285A, SSG62A0C950001, V1.0.0.0.8
4:: Siglent Technologies, SSG6285A, SSG62A0C950001, V1.0.0.0.8
5:: Siglent Technologies, SSG6285A, SSG62A0C950001, V1.0.0.0.8
6:: Siglent Technologies, SSG6285A, SSG62A0C950001, V1.0.0.0.8
7:: Siglent Technologies, SSG6285A, SSG62A0C950001, V1.0.0.0.8
8:: Siglent Technologies, SSG6285A, SSG62A0C950001, V1.0.0.0.8
9:: Siglent Technologies, SSG6285A, SSG62A0C950001, V1.0.0.0.8
Press "Enter" to exit
```



About SIGLENT

SIGLENT is an international high-tech company, concentrating on R&D, sales, production and services of electronic test & measurement instruments.

SIGLENT first began developing digital oscilloscopes independently in 2002. After more than a decade of continuous development, SIGLENT has extended its product line to include digital oscilloscopes, isolated handheld oscilloscopes, spectrum analyzers, function/arbitrary waveform generators, RF/MW signal generators, vector network analyzers, digital multimeters, DC power supplies, electronic loads and other general purpose test instrumentation. Since its first oscilloscope was launched in 2005, SIGLENT has become the fastest growing manufacturer of digital oscilloscopes. We firmly believe that today SIGLENT is the best value in electronic test & measurement

Headquarters:

SIGLENT Technologies Co., Ltd
Add: Bldg No.4 & No.5, Antongda Industrial Zone,
3rd Liuxian Road, Bao'an District,
Shenzhen, 518101, China
Tel: + 86 755 3688 7876
Fax: + 86 755 3359 1582
Email: sales@siglent.com
Website: int.siglent.com

North America:

SIGLENT Technologies NA, Inc
Add: 6557 Cochran Rd Solon, Ohio 44139
Tel: 440-398-5800
Toll Free: 877-515-5551
Fax: 440-399-1211
Email: support@siglentna.com
Website: www.siglentna.com

Europe:

SIGLENT Technologies Germany GmbH
Add: Staetzlinger Str. 70
86165 Augsburg, Germany
Tel: +49(0)-821-666 0 111 0
Fax: +49(0)-821-666 0 111 22
Email: info-eu@siglent.com
Website: www.siglenteu.com

Malaysia:

SIGLENT Technologies (M) Sdn.Bhd
Add: NO.6 Lorong Jelawat 4
Kawasan Perusahaan Seberang Jaya
13700, Perai Pulau Pinang
Tel: 006-04-3998964
Email: sales@siglent.com
Website: int.siglent.com

Follow us on
Facebook: **SiglentTech**

